

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020321\
 Data File : BG048104.D
 Acq On : 3 Feb 2021 23:39
 Operator : CG/JU
 Sample : M1291-12
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 OU421-008-0510

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG048104.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.667	389	396	405	rBV	807665	1272148	41.11%	8.060%
2	7.260	660	667	677	rBV	819848	1416264	45.76%	8.973%
3	8.118	806	813	819	rBV	170543	291470	9.42%	1.847%
4	9.275	1000	1010	1020	rVB	497764	882285	28.51%	5.590%
5	10.926	1283	1291	1300	rBV	236359	417472	13.49%	2.645%
6	13.364	1699	1706	1714	rVB	1286660	1966355	63.54%	12.459%
7	14.181	1840	1845	1850	rBV	40197	56948	1.84%	0.361%
8	14.739	1933	1940	1948	rVB	392356	637104	20.59%	4.037%
9	16.220	2184	2192	2203	rBV	1192132	1797120	58.07%	11.387%
10	17.477	2398	2406	2413	rBV	566306	857262	27.70%	5.432%
11	18.358	2551	2556	2575	rBV2	172281	290738	9.39%	1.842%
12	18.840	2634	2638	2644	rBV2	38809	60844	1.97%	0.386%
13	19.252	2704	2708	2716	rVB4	31111	47654	1.54%	0.302%
14	19.628	2767	2772	2783	rBV4	114003	239179	7.73%	1.515%
15	19.974	2825	2831	2837	rBV8	19677	36583	1.18%	0.232%
16	20.080	2843	2849	2855	rVB	2455948	3094764	100.00%	19.609%
17	20.556	2927	2930	2939	rBV3	26962	36156	1.17%	0.229%
18	21.079	3015	3019	3023	rBV4	18807	32380	1.05%	0.205%
19	21.384	3066	3071	3083	rBV2	170248	332914	10.76%	2.109%
20	21.749	3127	3133	3141	rBV	562510	939571	30.36%	5.953%
21	21.948	3163	3167	3173	rBV4	33335	48763	1.58%	0.309%
22	22.571	3269	3273	3276	rBV4	29833	51444	1.66%	0.326%
23	25.027	3681	3691	3704	rVB2	329677	977346	31.58%	6.192%




Sum of corrected areas: 15782764

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020321\
Data File : BG048104.D
Acq On : 3 Feb 2021 23:39
Operator : CG/JU
Sample : M1291-12
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU421-008-0510

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

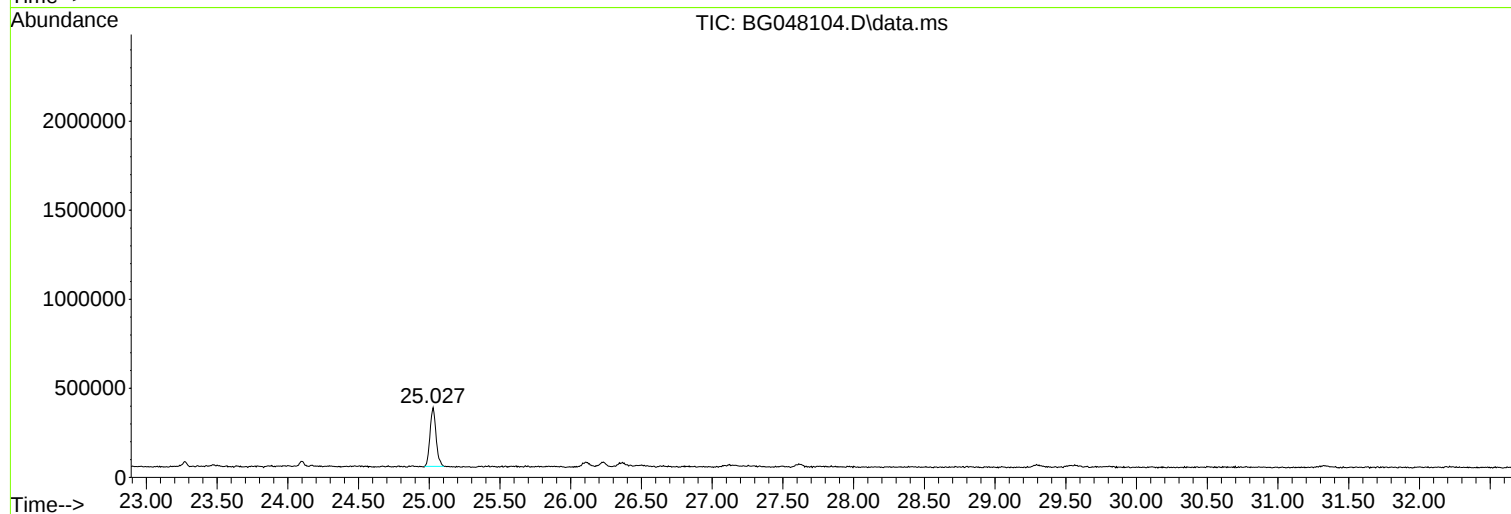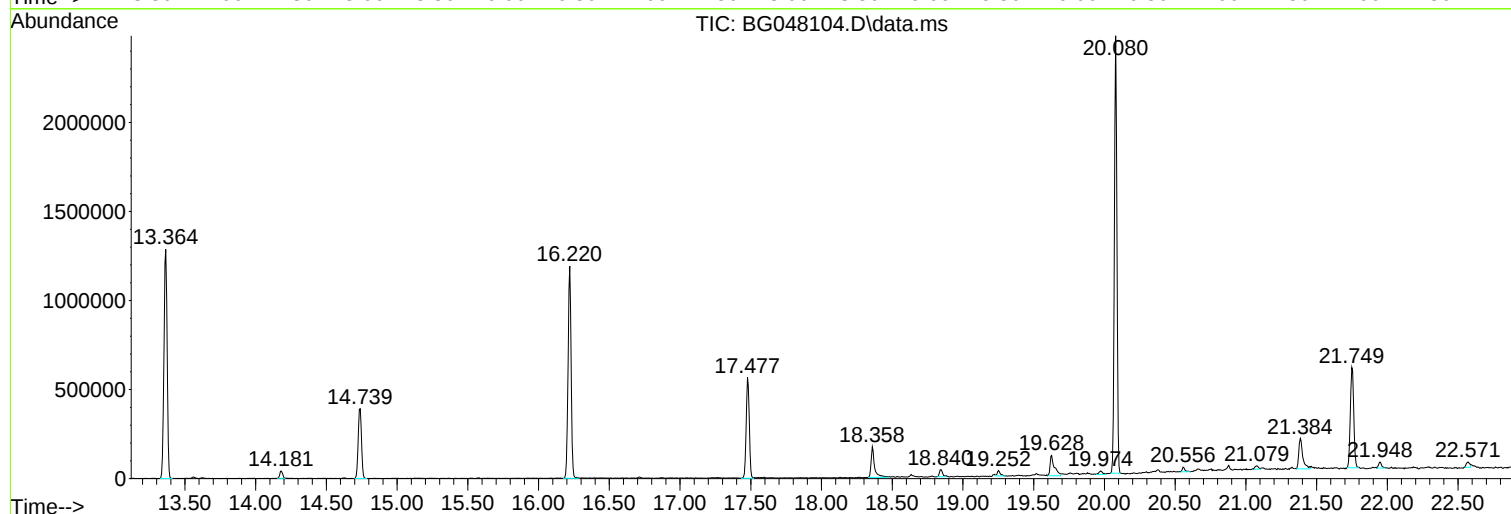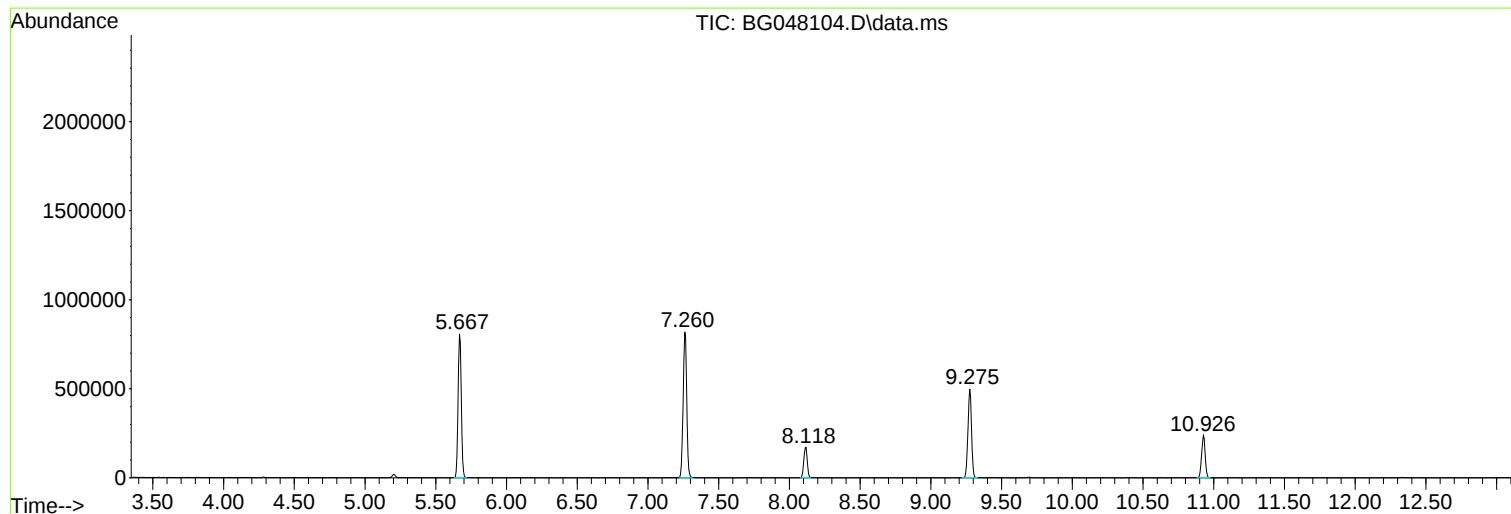

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020321\
Data File : BG048104.D
Acq On : 3 Feb 2021 23:39
Operator : CG/JU
Sample : M1291-12
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU421-008-0510

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020321\
Data File : BG048104.D
Acq On : 3 Feb 2021 23:39
Operator : CG/JU
Sample : M1291-12
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
OU421-008-0510

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------