
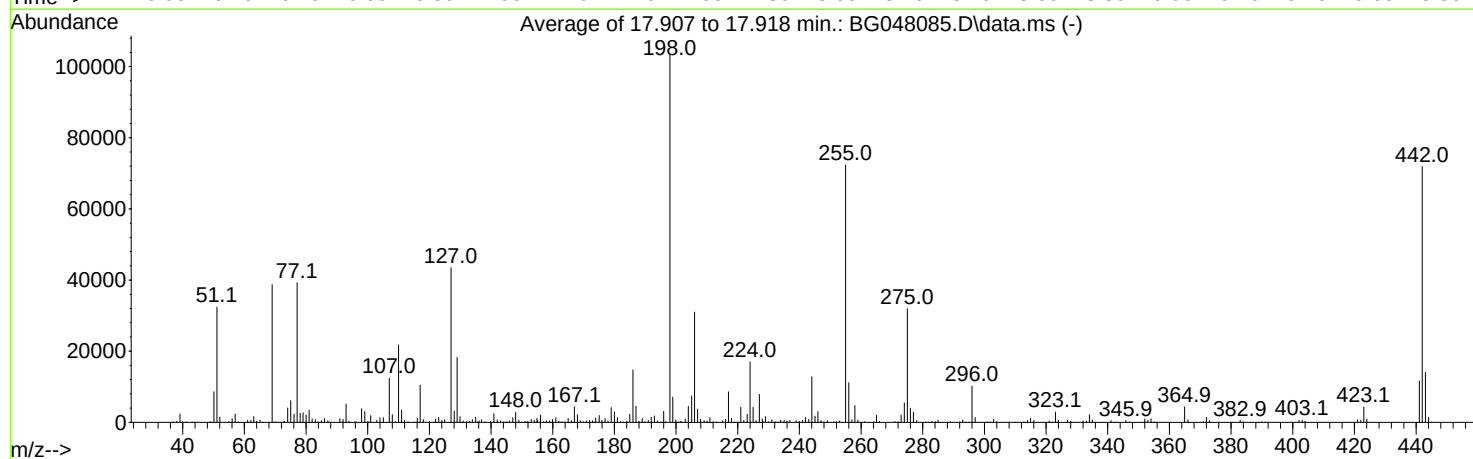


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG020321\  
 Data File : BG048085.D  
 Acq On : 3 Feb 2021 9:58  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG012521.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Feb 02 15:30:13 2021

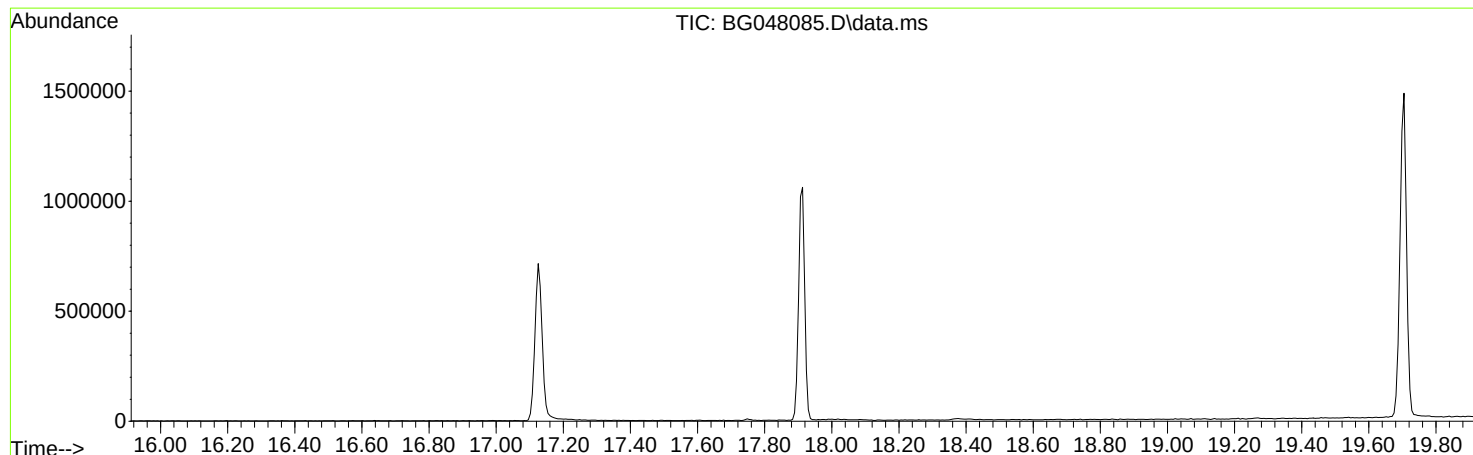

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 31.3         | 32400      | PASS                |
| 68             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 69             | 198             | 0.00            | 100             | 37.4         | 38712      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 186        | PASS                |
| 127            | 198             | 10              | 80              | 42.1         | 43507      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 103395     | PASS                |
| 199            | 198             | 5               | 9               | 6.9          | 7092       | PASS                |
| 275            | 198             | 10              | 60              | 30.9         | 31912      | PASS                |
| 365            | 198             | 1               | 100             | 4.2          | 4370       | PASS                |
| 441            | 198             | 0.01            | 100             | 11.3         | 11666      | PASS                |
| 442            | 198             | 50              | 100             | 69.5         | 71904      | PASS                |
| 443            | 442             | 15              | 24              | 19.6         | 14062      | PASS                |

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP




# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 2/3/2021      | BNA_G            | <u>BG048085.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 430906           | 20.938             |
| DDD           | 3227             | 20.492             |
| DDE           | 527              | 19.987             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 3754          | 434660           | 0.86               |
|               |                  |                    |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG020321\  
 Data File : BG048085.D  
 Acq On : 3 Feb 2021 9:58  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Quant Time: Feb 04 01:11:50 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG012521.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Feb 02 15:30:13 2021  
 Response via : Initial Calibration

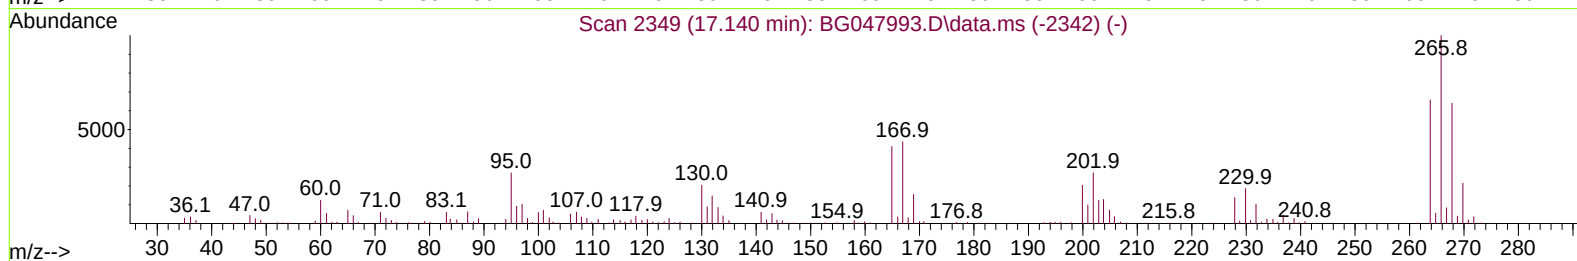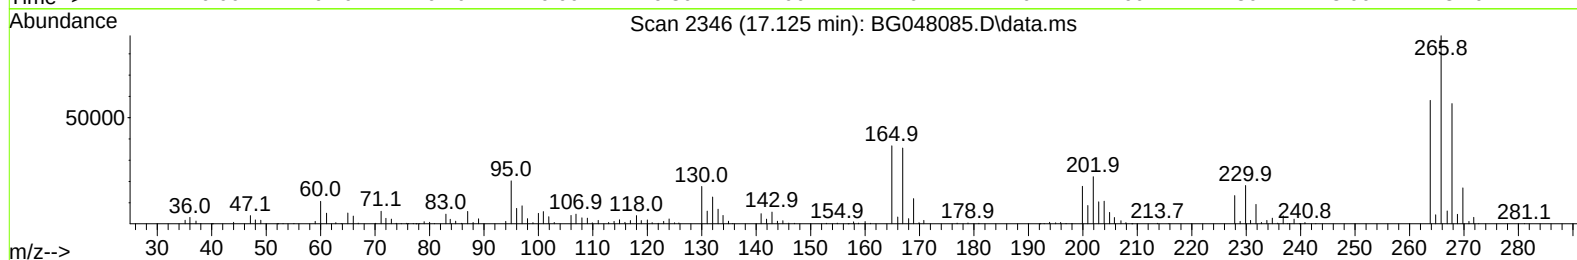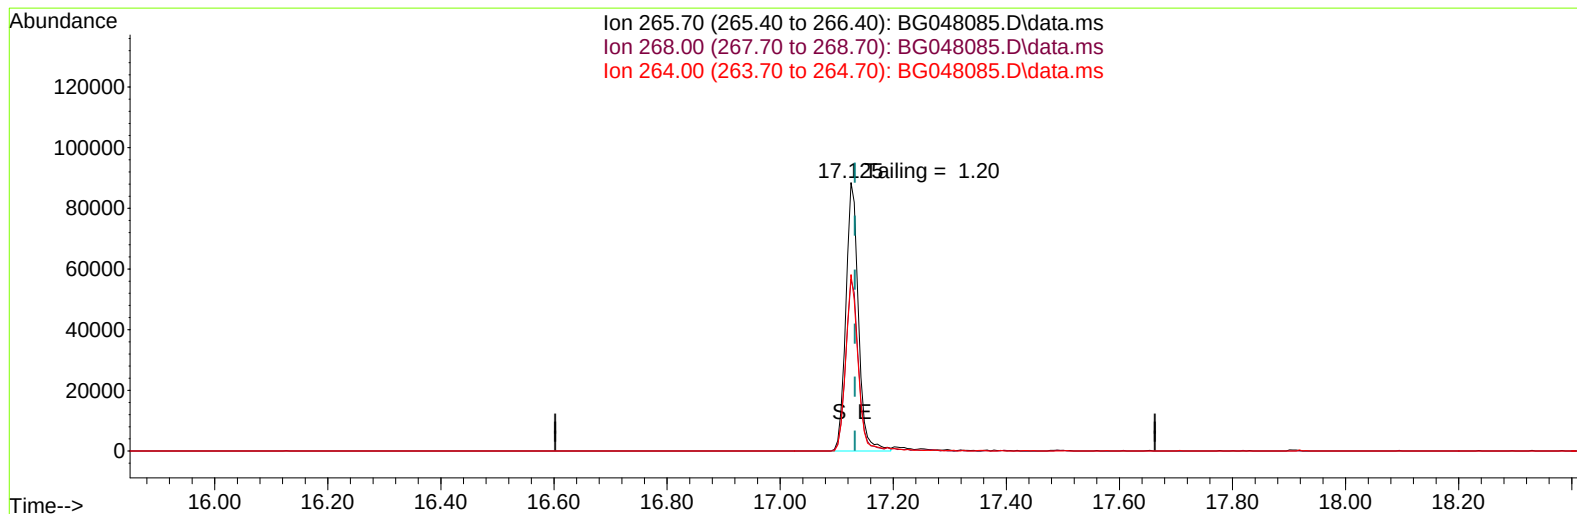

TIC: BG048085.D\data.ms

**(70) Pentachlorophenol (C)**

17.125min (-0.007) 35422.42 ng




response 136901

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 63.96  |
| 264.00 | 61.60  | 65.68  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG020321\  
 Data File : BG048085.D  
 Acq On : 3 Feb 2021 9:58  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Quant Time: Feb 04 01:11:50 2021  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG012521.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Feb 02 15:30:13 2021  
 Response via : Initial Calibration

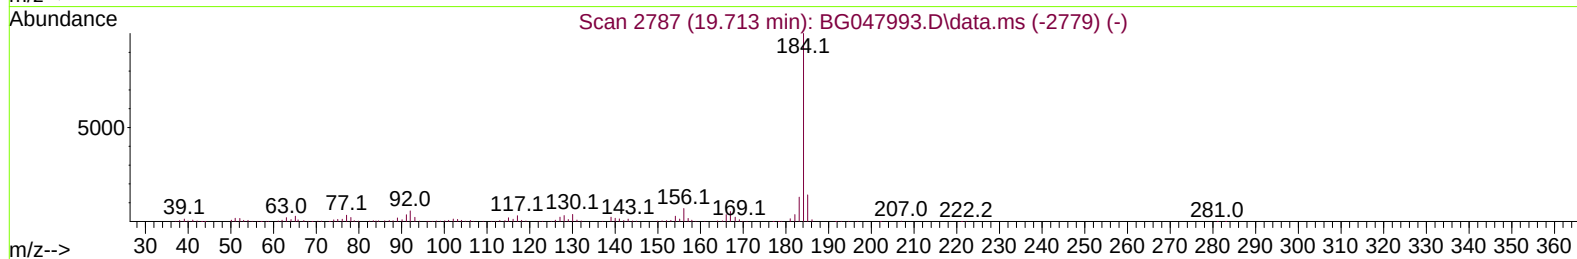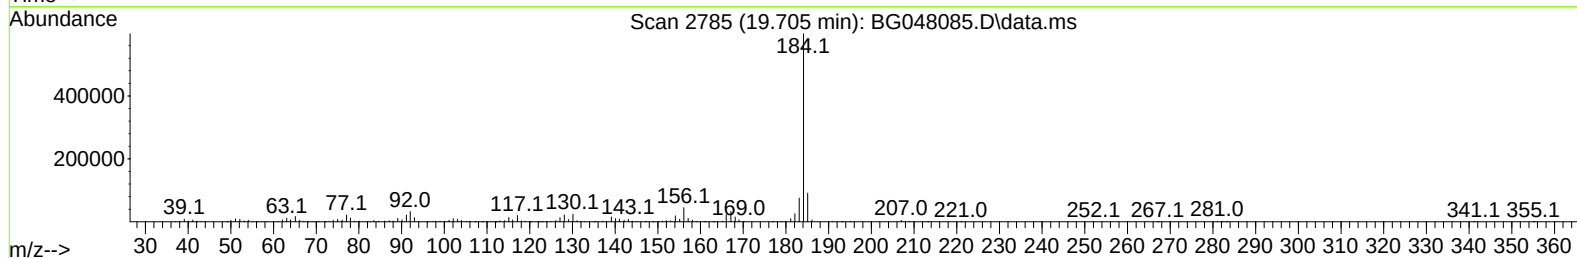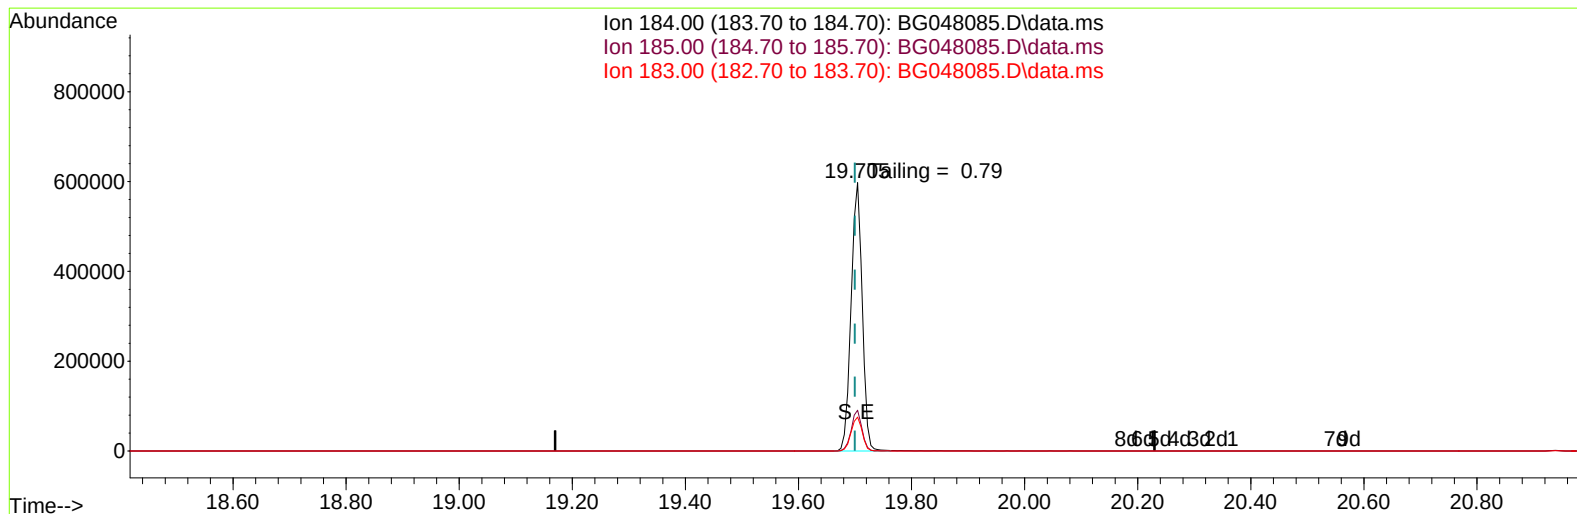

TIC: BG048085.D\data.ms

**(77) Benzidine**

19.705min (+ 0.004) 533516.23 ng m

response 815716

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 15.24  |
| 183.00 | 13.20  | 12.64  |
| 0.00   | 0.00   | 0.00   |