
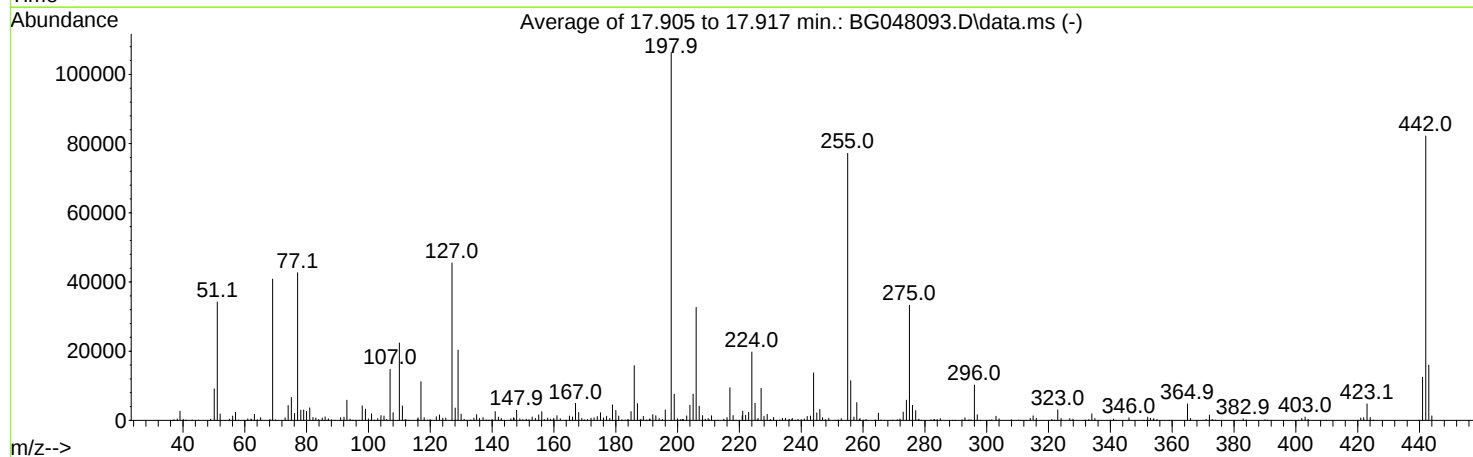


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020321\
 Data File : BG048093.D
 Acq On : 3 Feb 2021 16:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 02 15:30:13 2021

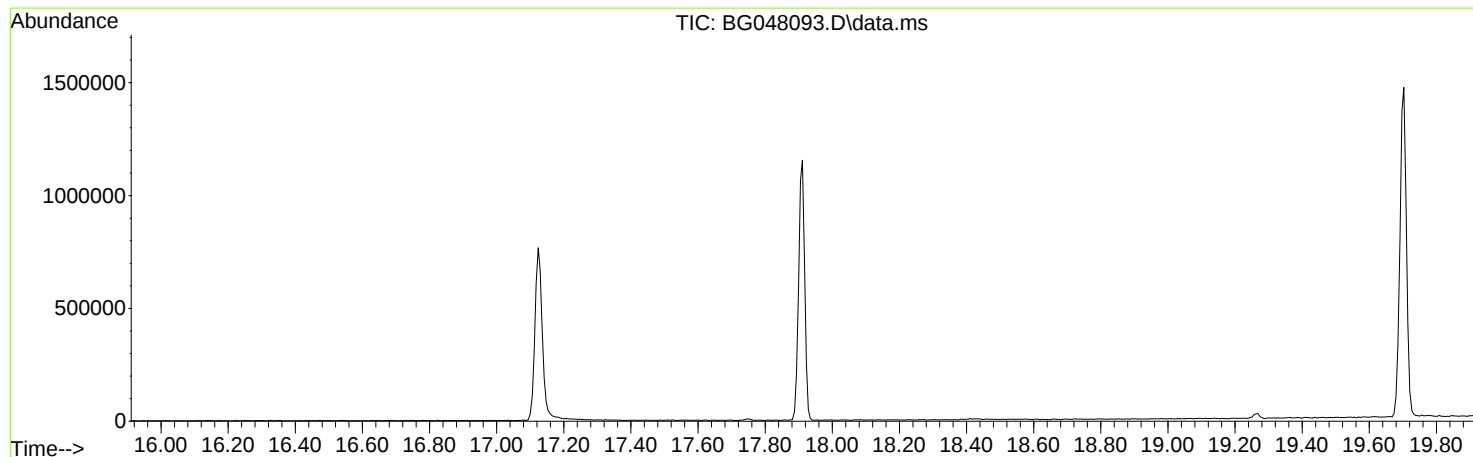

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	34208	PASS
68	69	0.00	2	0.7	292	PASS
69	198	0.00	100	38.4	40824	PASS
70	69	0.00	2	0.4	162	PASS
127	198	10	80	42.8	45501	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	106336	PASS
199	198	5	9	7.1	7573	PASS
275	198	10	60	31.3	33267	PASS
365	198	1	100	4.5	4789	PASS
441	198	0.01	100	11.7	12433	PASS
442	198	50	100	77.3	82171	PASS
443	442	15	24	19.4	15968	PASS

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/3/2021	BNA_G	<u>BG048093.D</u>
Compound Name	Response	Retention Time
DDT	452061	20.937
DDD	3728	20.49
DDE	575	19.985
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4303	456364	0.94

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020321\
Data File : BG048093.D
Acq On : 3 Feb 2021 16:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 04 01:18:03 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 02 15:30:13 2021
Response via : Initial Calibration

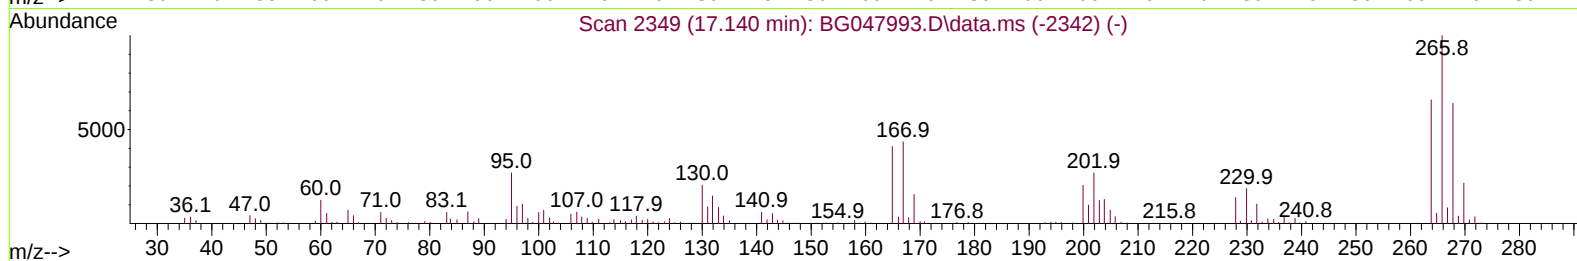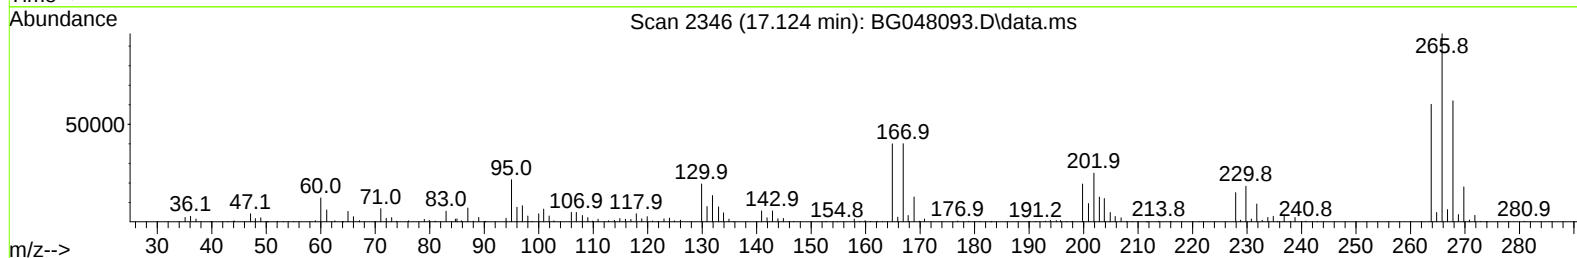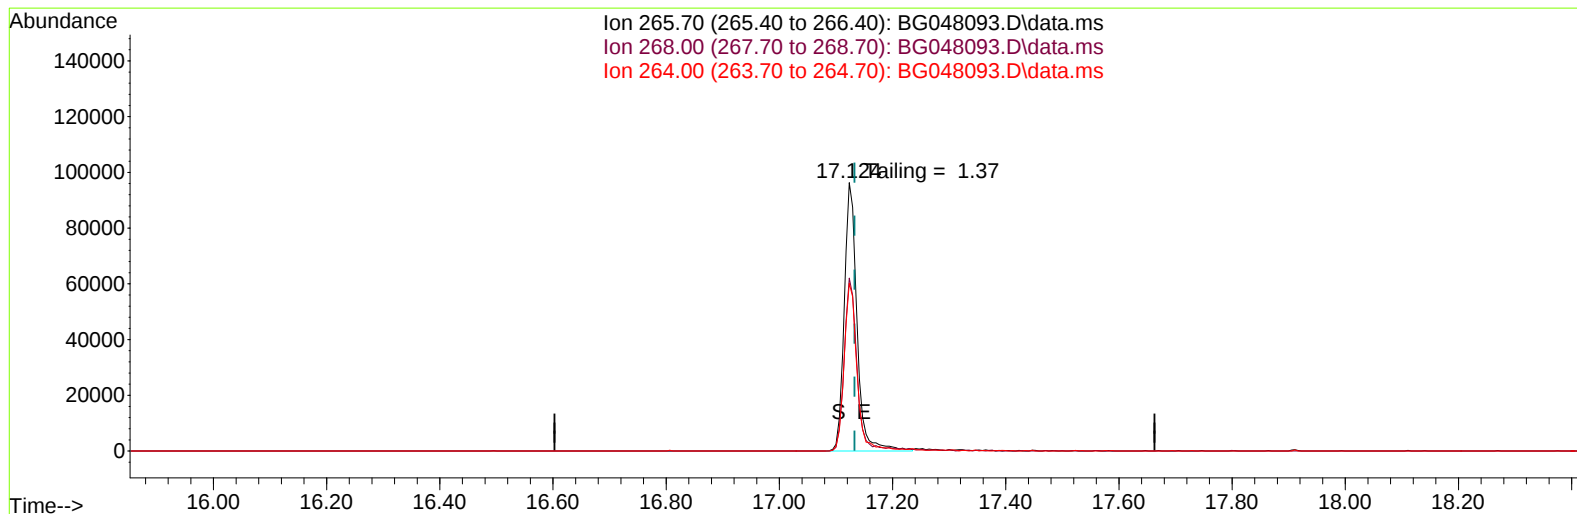

TIC: BG048093.D\data.ms

(70) Pentachlorophenol (C)

17.124min (-0.009) 317740.19 ng




response 151398

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.43
264.00	61.60	62.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020321\
 Data File : BG048093.D
 Acq On : 3 Feb 2021 16:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Feb 04 01:18:03 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 02 15:30:13 2021
 Response via : Initial Calibration

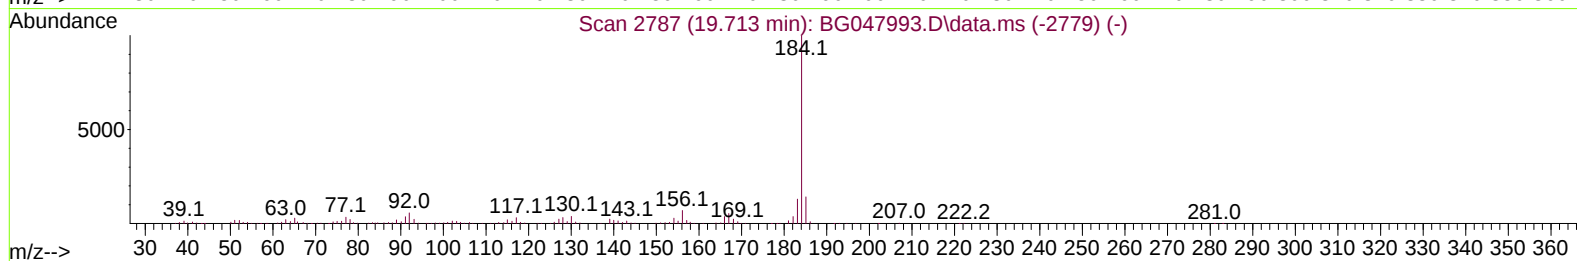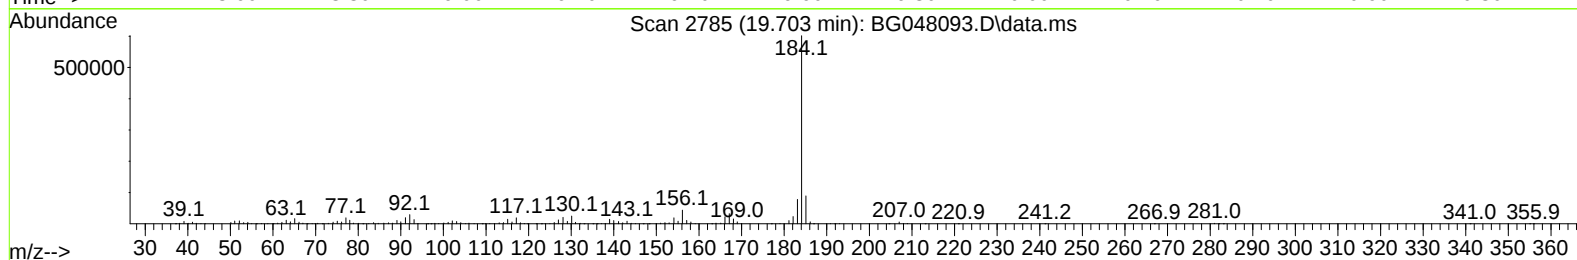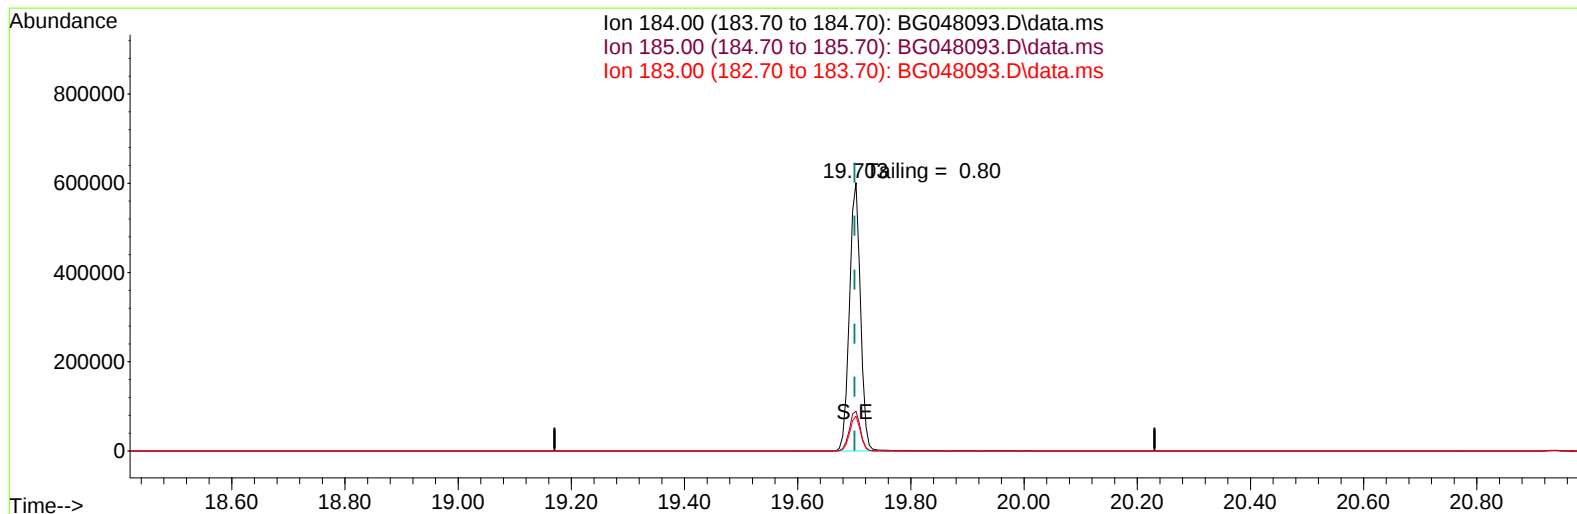

TIC: BG048093.D\data.ms

(77) Benzidine

19.703min (+ 0.003) 4352.04 ng m

response 810786

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.87
183.00	13.20	12.96
0.00	0.00	0.00