
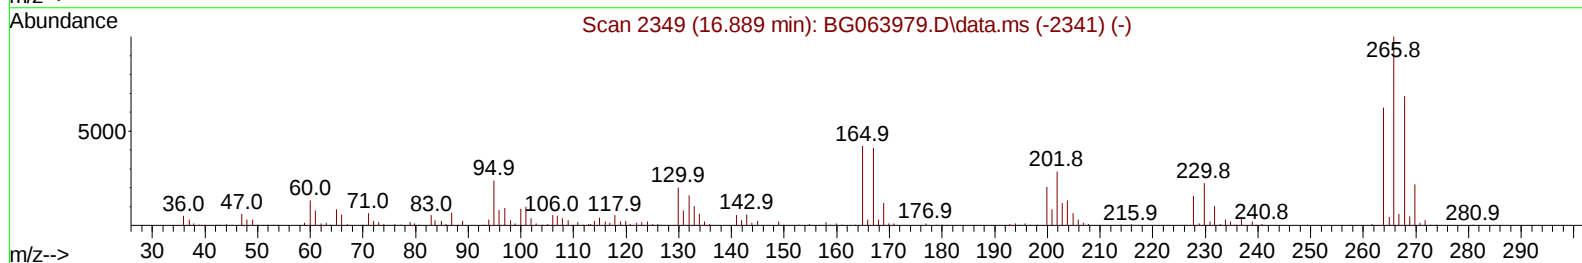
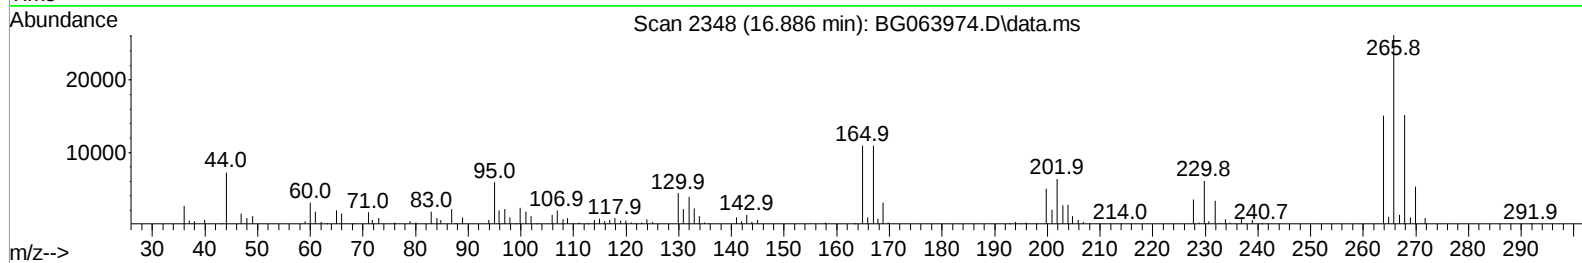


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020325\
Data File : BG063974.D
Acq On : 3 Feb 2025 10:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 02:35:06 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 04 02:30:48 2025
Response via : Initial Calibration

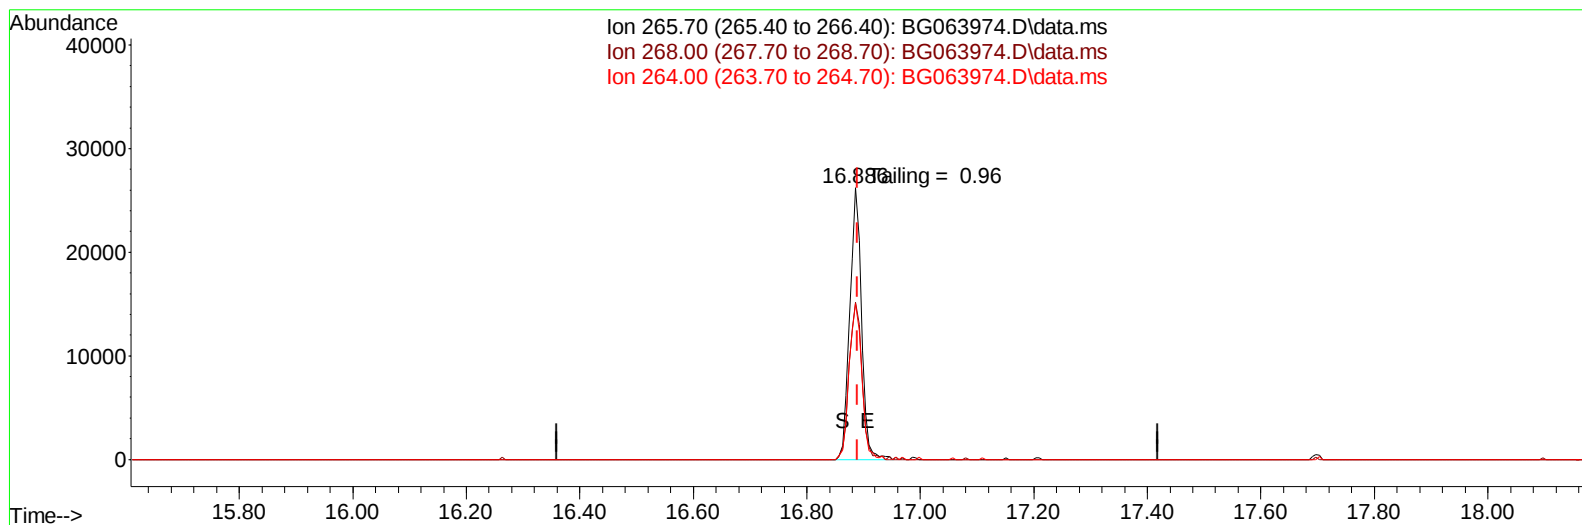

TIC: BG063974.D\data.ms

(70) Pentachlorophenol (C)




16.886min (-0.003) 74371.74 ng

response 37632

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.50	57.98
264.00	62.50	57.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020325\
Data File : BG063974.D
Acq On : 3 Feb 2025 10:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 02:35:06 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 04 02:30:48 2025
Response via : Initial Calibration

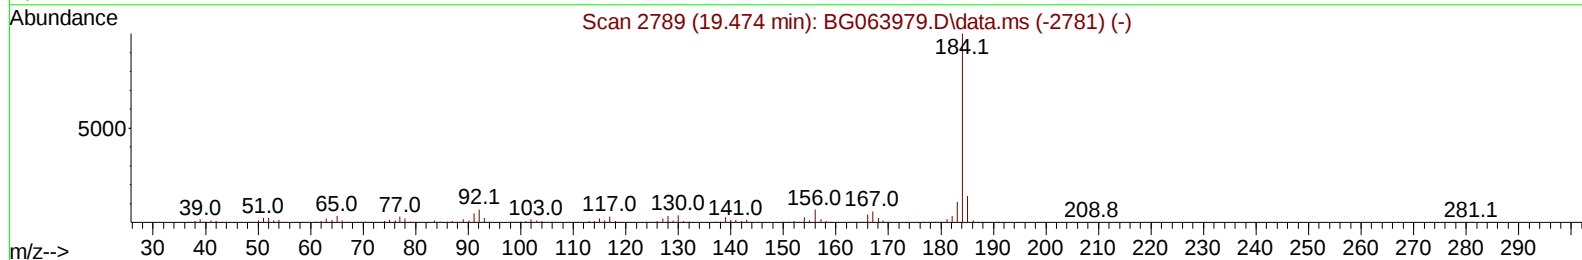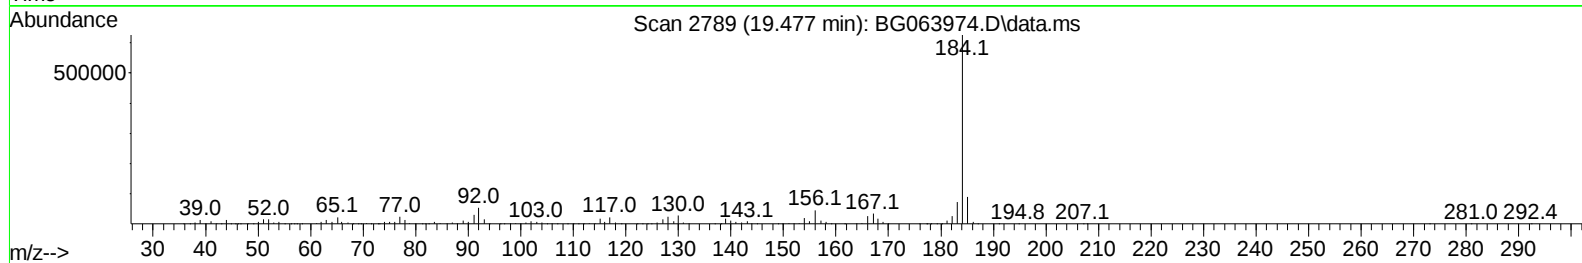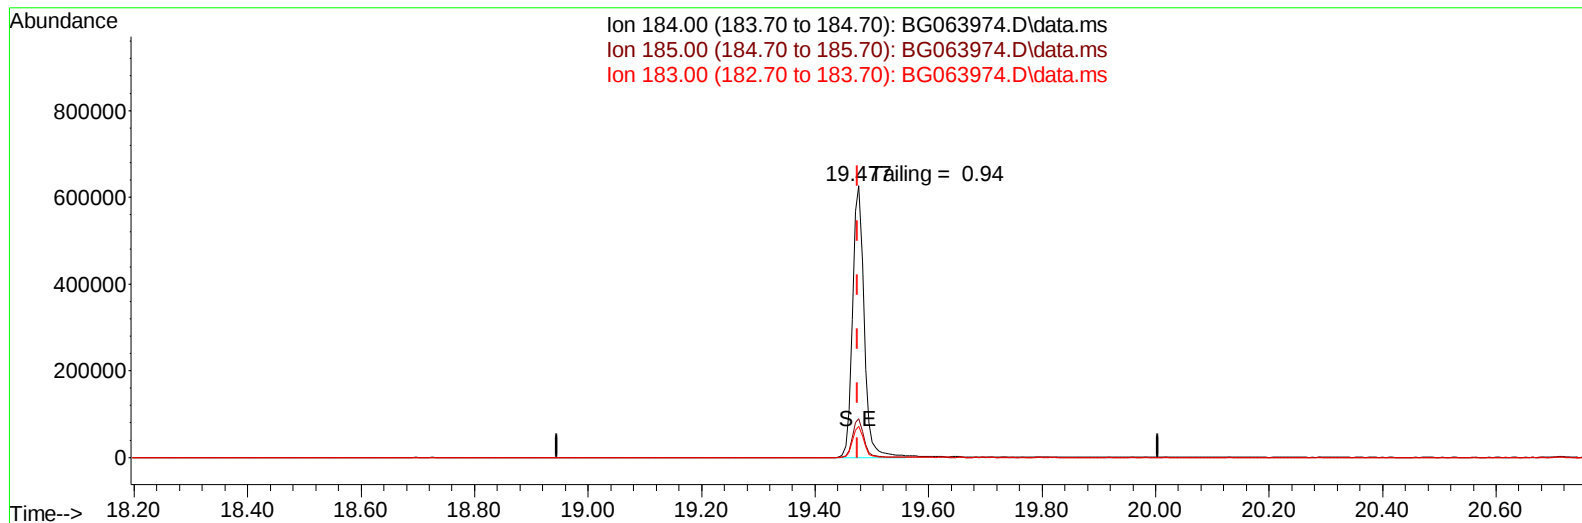

TIC: BG063974.D\data.ms

(77) Benzidine**19.477min (+ 0.003) 7478.24 ng****response 894155**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.19
183.00	10.90	11.51
0.00	0.00	0.00