

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG020416\
 Data File : BG020788.D
 Acq On : 4 Feb 2016 15:51
 Operator : SJ/IZ
 Sample : H1334-16
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBG13

Quant Time: Feb 05 04:19:57 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG012716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 05 04:10:17 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.28	152	19540	20.00	ng/ul	0.00
18) Naphthalene-d8	11.10	136	98618	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.89	164	56386	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.62	188	108640	20.00	ng/ul	0.00
78) Chrysene-d12	21.90	240	90811	20.00	ng/ul	0.00
86) Perylene-d12	25.29	264	87934	20.00	ng/ul	0.02

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.62	96	1110	2.72	ng/uL	0.00
5) Phenol-d5	7.41	99	30501	15.25	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.59	67	17851	17.13	ng/ul	0.00
9) 2-Chlorophenol-d4	7.80	132	25842	17.21	ng/ul	0.00
13) 4-Methylphenol-d8	8.97	113	26107	15.13	ng/ul	0.00
19) Nitrobenzene-d5	9.45	128	12476	20.73	ng/ul	0.00
22) 2-Nitrophenol-d4	10.17	143	10626	20.14	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.71	165	24929	17.31	ng/ul	0.00
29) 4-Chloroaniline-d4	11.23	131	34655	17.11	ng/ul	0.00
44) Dimethylphthalate-d6	14.28	166	85318	17.71	ng/ul	0.00
47) Acenaphthylene-d8	14.59	160	112957	19.24	ng/ul	0.00
52) 4-Nitrophenol-d4	15.05	143	10229	12.01	ng/ul	0.00
58) Fluorene-d10	15.87	176	74993	17.81	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.97	200	4565	12.72	ng/ul	0.00
71) Anthracene-d10	17.72	188	103005	19.28	ng/ul	0.00
79) Pyrene-d10	19.99	212	95421	19.36	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.05	264	91604	19.44	ng/ul	0.00

Target Compounds


						Qvalue
45) Dimethylphthalate	14.33	163	25887	5.15	ng/ul#	98
70) Phenanthrene	17.66	178	28719	4.21	ng/ul	97
72) Anthracene	17.66	178	28719	4.21	ng/ul	96
77) Fluoranthene	19.65	202	56034	7.99	ng/ul#	76
80) Pyrene	20.01	202	44538	6.49	ng/ul#	76
83) Benzo(a)anthracene	21.88	228	23852	4.08	ng/ul	98
85) Chrysene	21.88	228	23852	4.39	ng/ul	99
88) Benzo(b)fluoranthene	24.20	252	26942	4.68	ng/ul#	90
89) Benzo(k)fluoranthene	24.20	252	26942	4.77	ng/ul#	90
91) Benzo(a)pyrene	25.12	252	18636	3.38	ng/ul#	83
92) Indeno(1,2,3-cd)pyrene	29.14	276	13380	2.08	ng/ul#	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG020416\
Data File : BG020788.D
Acq On : 4 Feb 2016 15:51
Operator : SJ/IZ
Sample : H1334-16
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BBG13

Quant Time: Feb 05 04:19:57 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG012716.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 05 04:10:17 2016
Response via : Initial Calibration




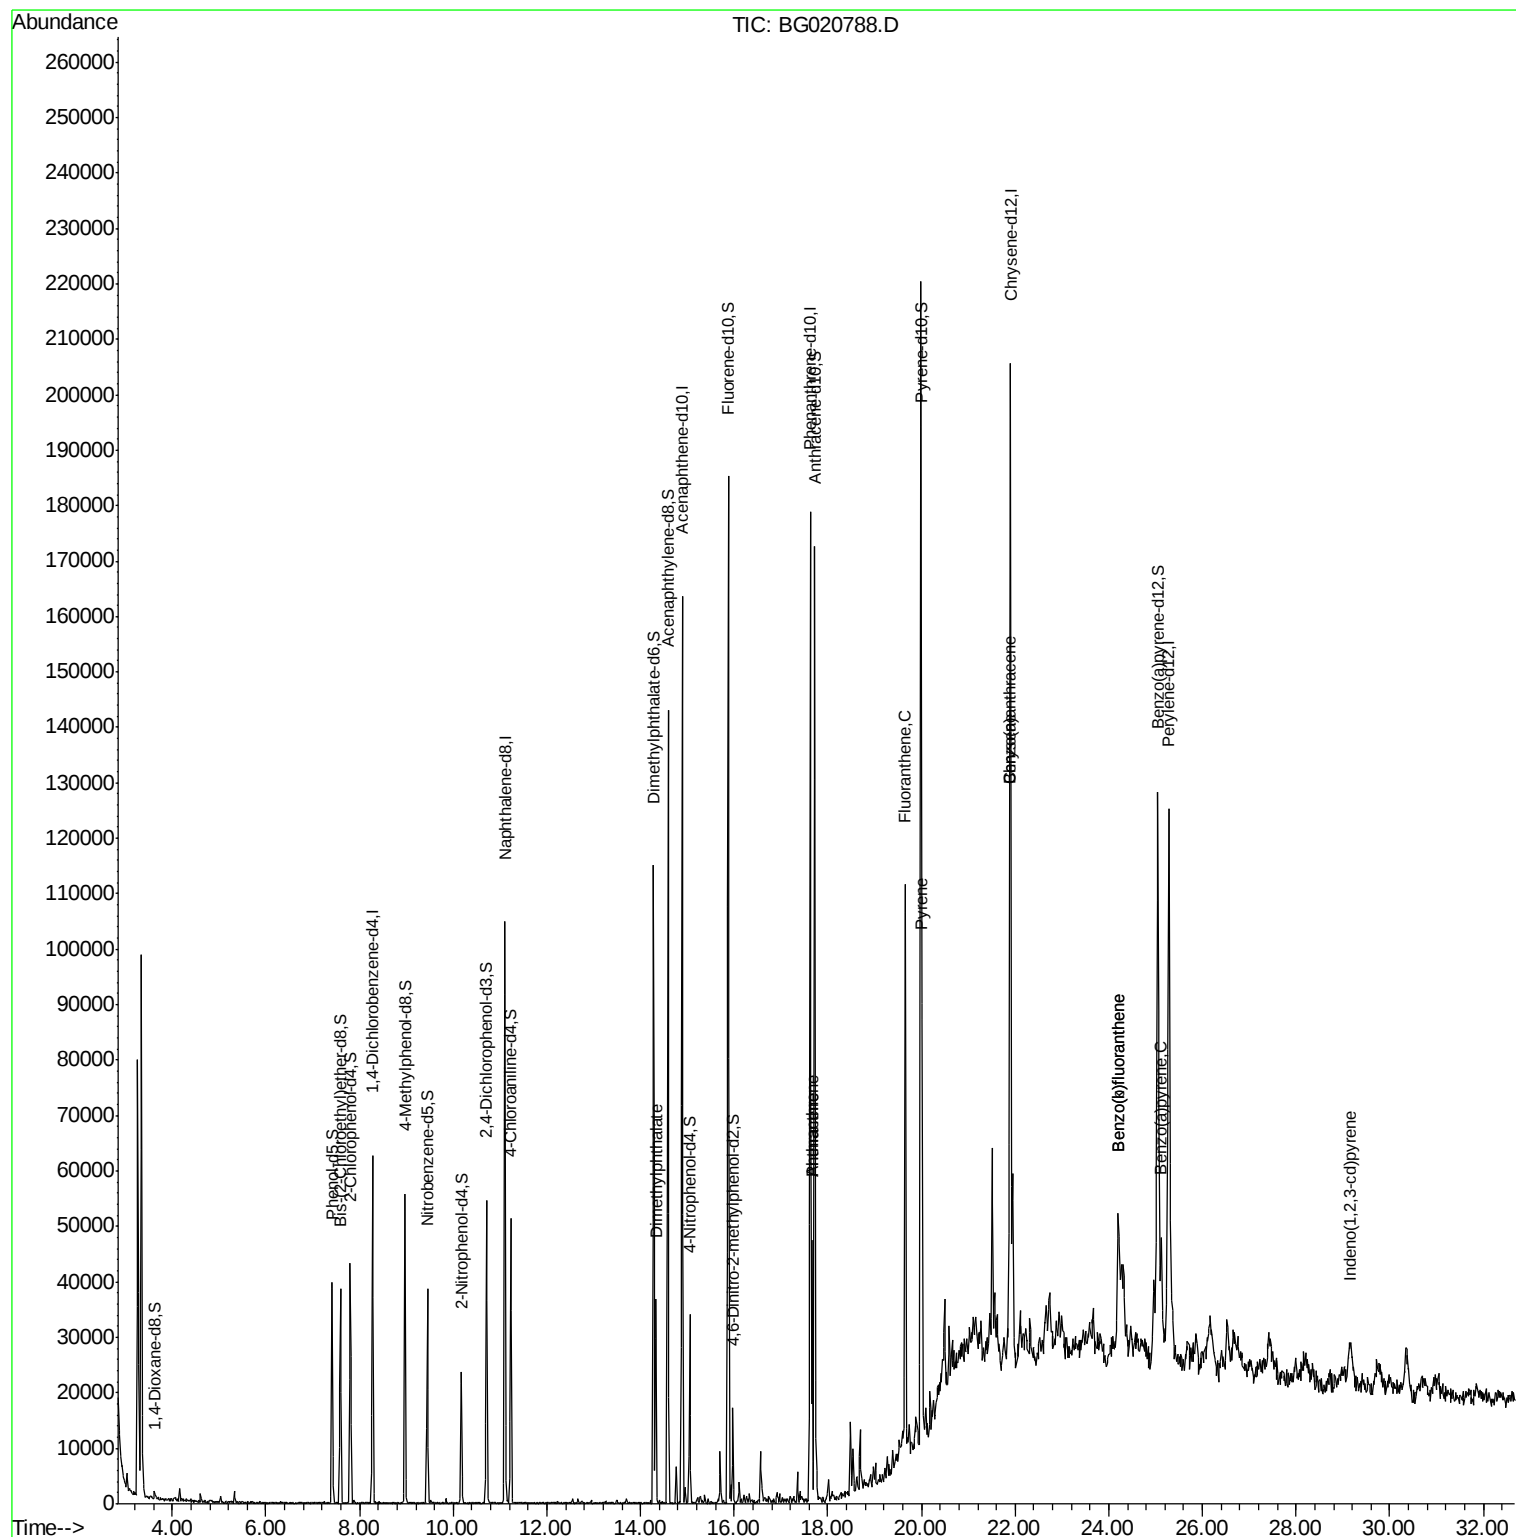


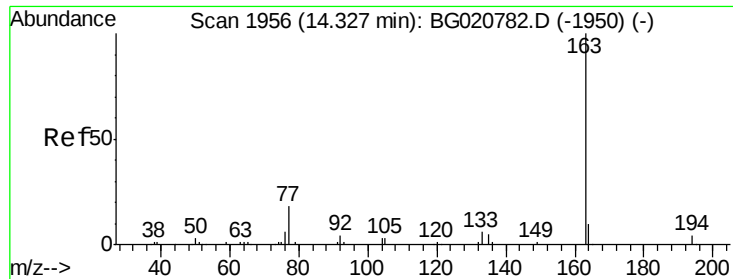

#45
Dimethylphthalate
Concen: 5.15 ng/ul
RT: 14.33 min Scan# 1956
Delta R.T. 0.00 min
Lab File: BG020788.D
Acq: 4 Feb 2016 15:51




Instrument :
BNA_G
ClientSampleId :
BBG13


Tgt Ion:163 Resp: 25887
Ion Ratio Lower Upper
163 100
194 3.6 4.0 6.0#
164 11.0 8.4 12.6

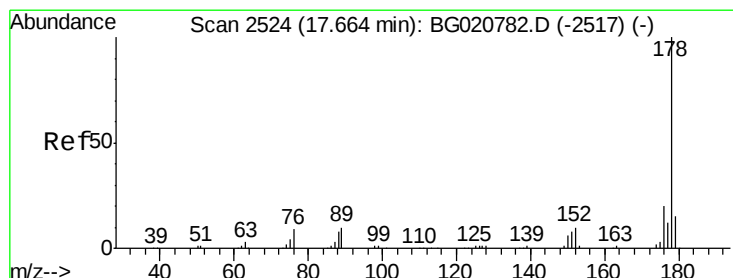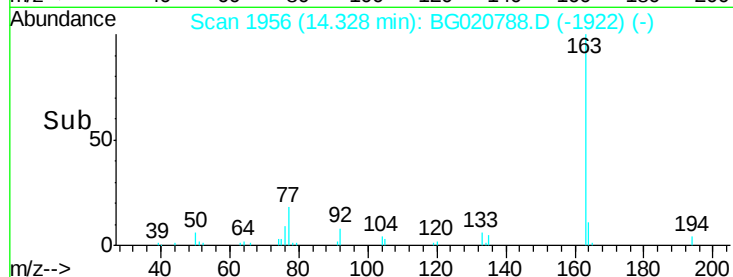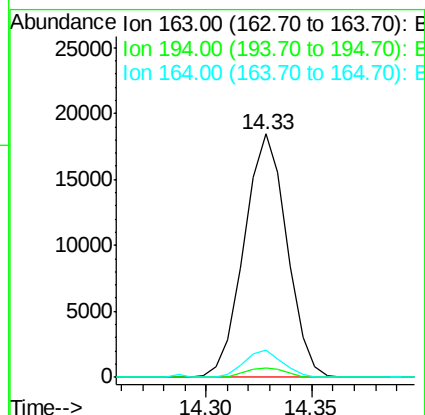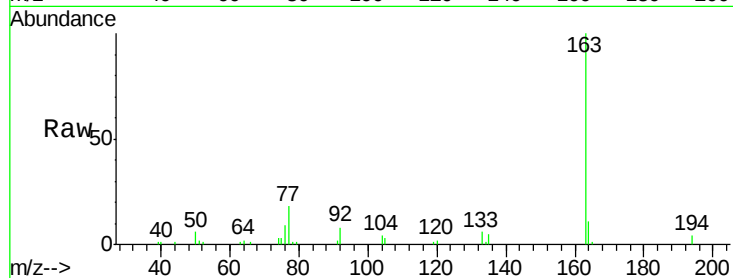

#70
Phenanthrene
Concen: 4.21 ng/ul
RT: 17.66 min Scan# 2524
Delta R.T. 0.00 min
Lab File: BG020788.D
Acq: 4 Feb 2016 15:51

Tgt Ion:178 Resp: 28719
Ion Ratio Lower Upper
178 100
179 13.8 12.3 18.5
176 20.2 15.4 23.0

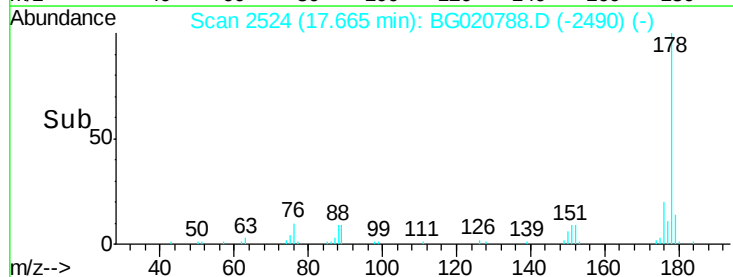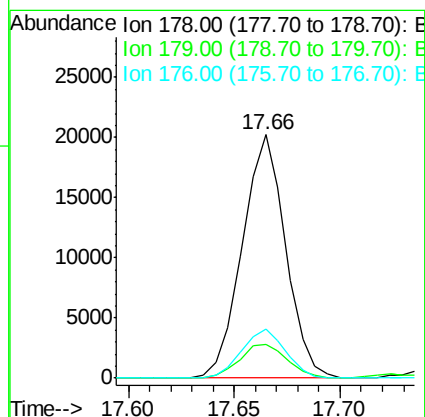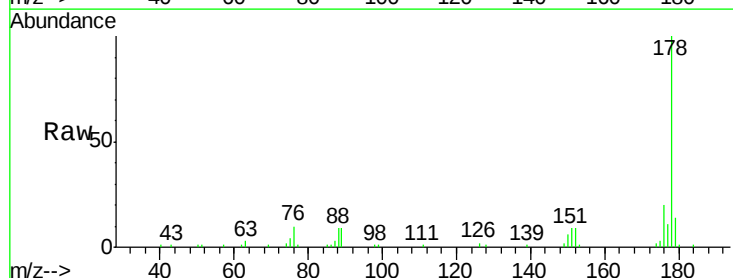

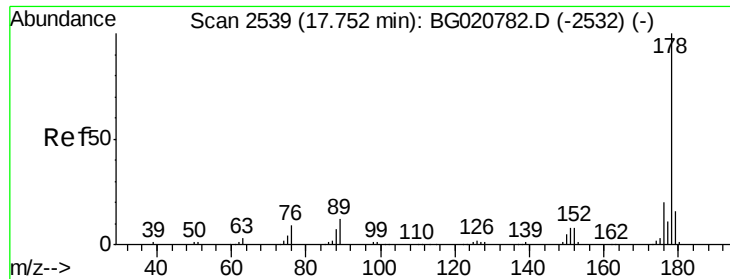

#72

Anthracene

Concen: 4.21 ng/ul

RT: 17.66 min Scan# 2524

Delta R.T. -0.09 min

Lab File: BG020788.D

Acq: 4 Feb 2016 15:51

Instrument :

BNA_G

ClientSampleId :

BBG13


Tgt Ion:178 Resp: 28719

Ion Ratio Lower Upper

178 100

179 13.8 13.4 20.2




176 20.2 15.4 23.0

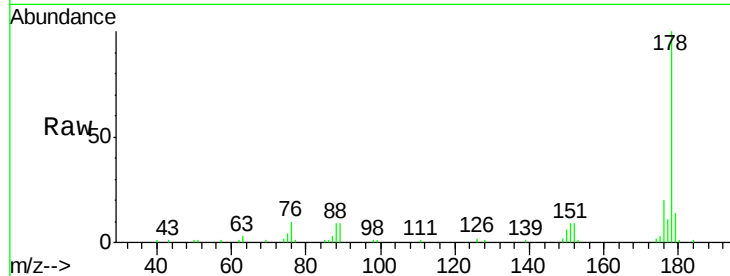

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

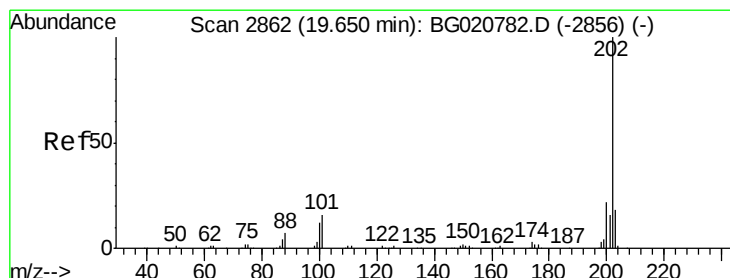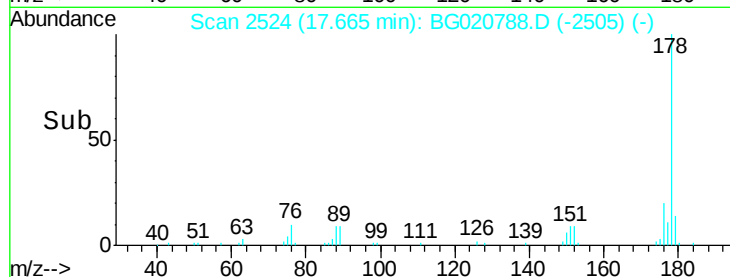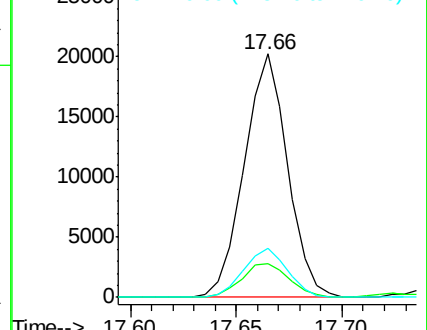

#77

Fluoranthene

Concen: 7.99 ng/ul

RT: 19.65 min Scan# 2862

Delta R.T. 0.00 min

Lab File: BG020788.D

Acq: 4 Feb 2016 15:51


Tgt Ion:202 Resp: 56034

Ion Ratio Lower Upper

202 100

101 16.6 6.1 9.1#



100 13.1 4.6 7.0#

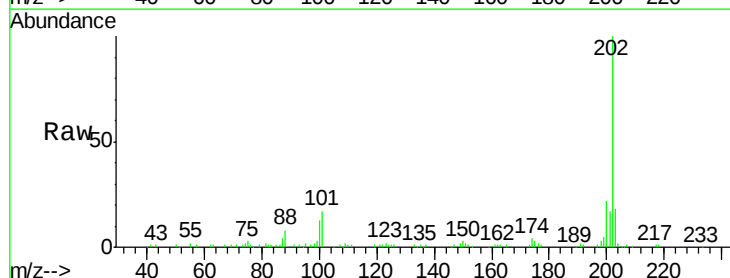


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B



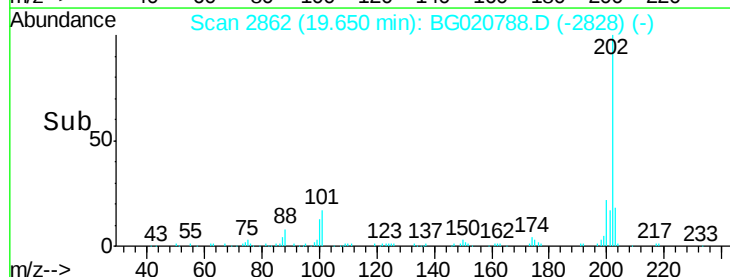
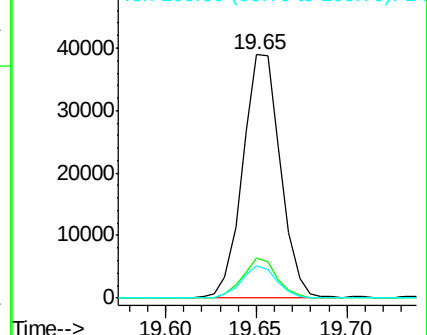


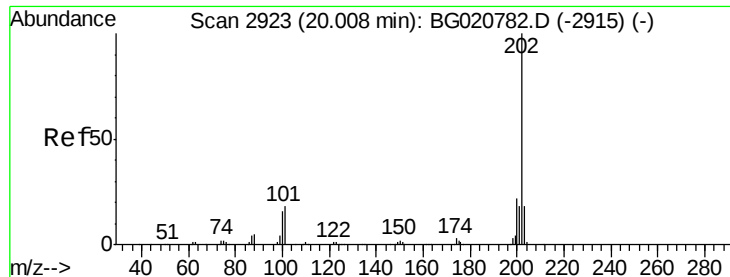

#80
 Pyrene
 Concen: 6.49 ng/ul
 RT: 20.01 min Scan# 2924
 Delta R.T. 0.01 min
 Lab File: BG020788.D
 Acq: 4 Feb 2016 15:51




Instrument :
 BNA_G
 ClientSampleId :
 BBG13


Tgt Ion:202 Resp: 44538
 Ion Ratio Lower Upper
 202 100
 101 16.2 6.9 10.3#
 100 16.3 5.6 8.4#

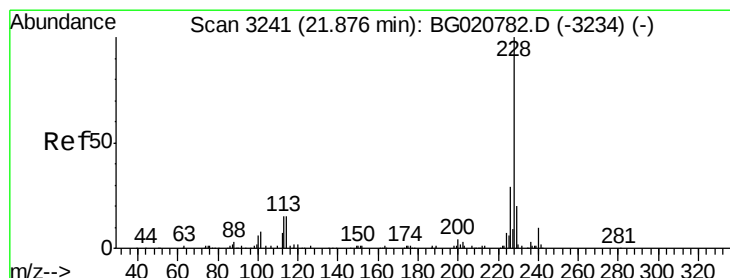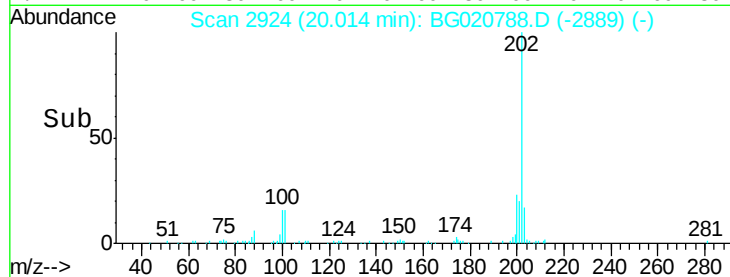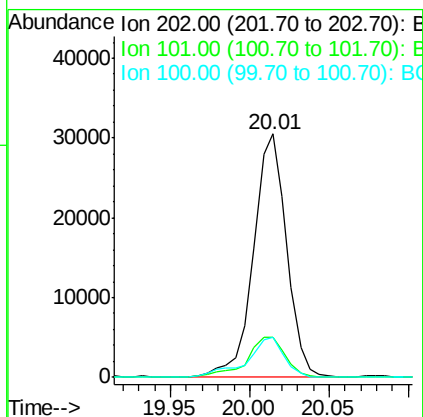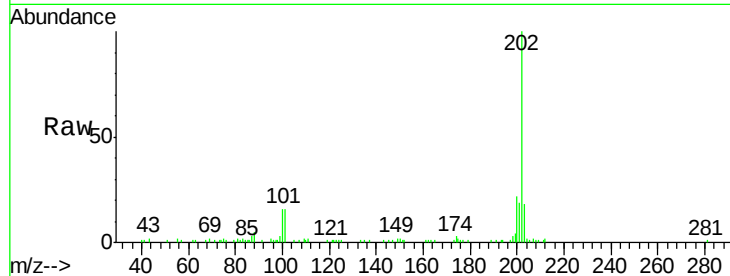

#83
 Benzo(a)anthracene
 Concen: 4.08 ng/ul
 RT: 21.88 min Scan# 3241
 Delta R.T. 0.00 min
 Lab File: BG020788.D
 Acq: 4 Feb 2016 15:51

Tgt Ion:228 Resp: 23852
 Ion Ratio Lower Upper
 228 100
 229 20.4 16.0 24.0
 226 29.1 21.8 32.8

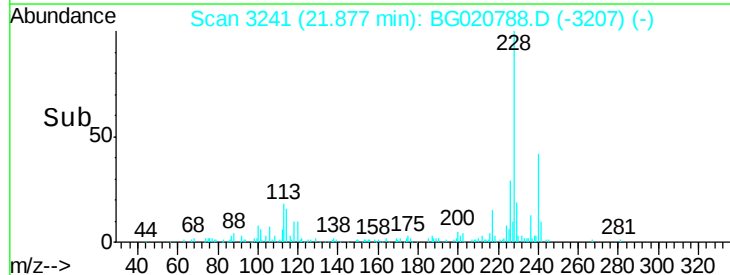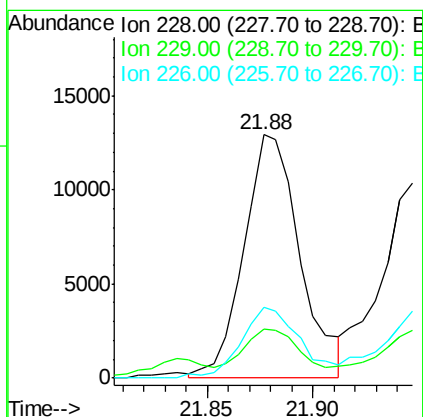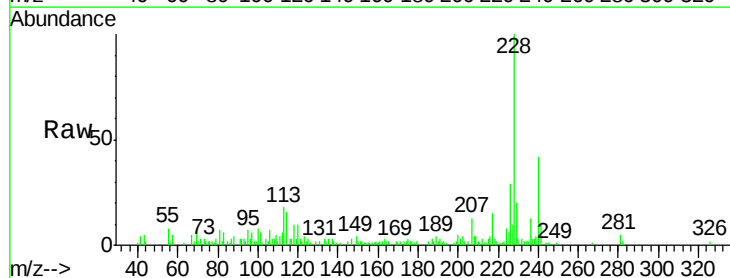

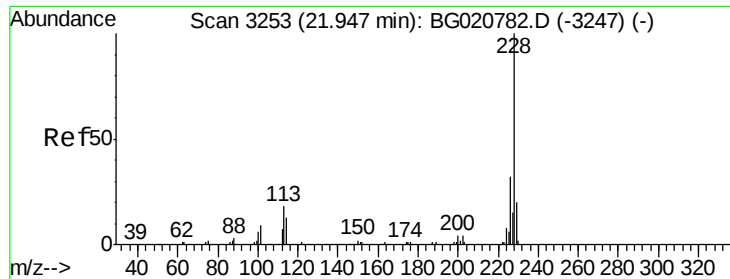

#85

Chrysene

Concen: 4.39 ng/ul

RT: 21.88 min Scan# 3241

Delta R.T. -0.07 min

Lab File: BG020788.D

Acq: 4 Feb 2016 15:51

Instrument :

BNA_G

ClientSampleId :

BBG13


Tgt Ion:228 Resp: 23852

Ion Ratio Lower Upper

228 100

226 29.1 24.1 36.1




229 20.4 16.0 24.0

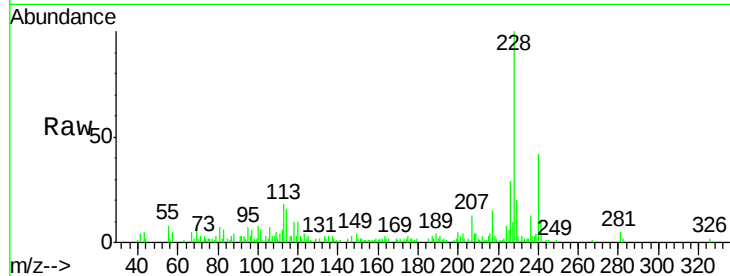

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

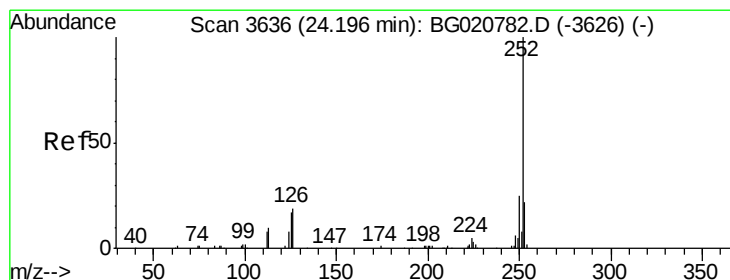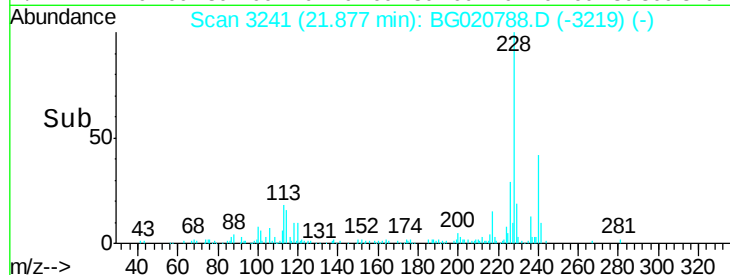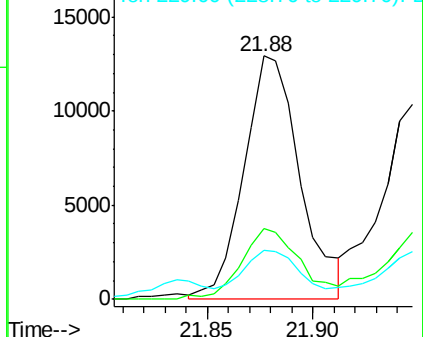

#88

Benzo(b)fluoranthene

Concen: 4.68 ng/ul

RT: 24.20 min Scan# 3637

Delta R.T. 0.01 min

Lab File: BG020788.D

Acq: 4 Feb 2016 15:51


Tgt Ion:252 Resp: 26942

Ion Ratio Lower Upper

252 100

253 21.6 17.4 26.0



125 20.6 4.9 7.3#

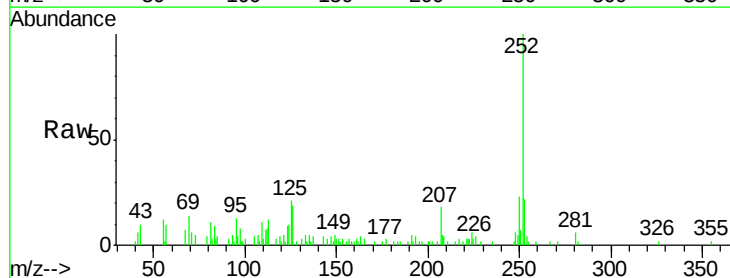


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

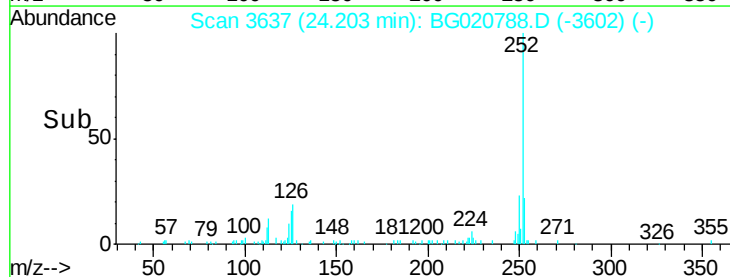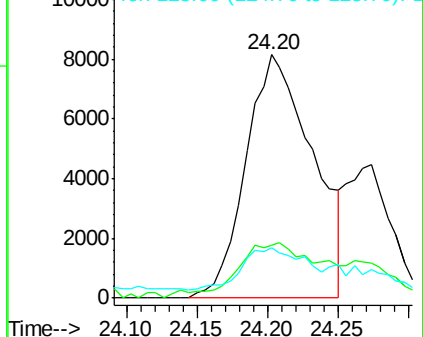

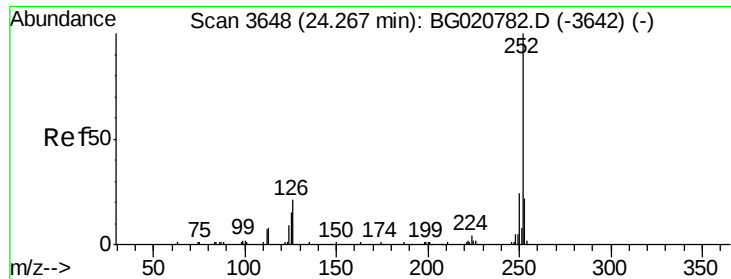

#89

Benzo(k)fluoranthene

Concen: 4.77 ng/ul

RT: 24.20 min Scan# 3637

Delta R.T. -0.06 min

Lab File: BG020788.D

Acq: 4 Feb 2016 15:51

Instrument :

BNA_G

ClientSampleId :

BBG13





Tgt Ion:252 Resp: 26942

Ion Ratio Lower Upper

252 100

253 21.6 17.1 25.7

125 20.6 5.4 8.0#

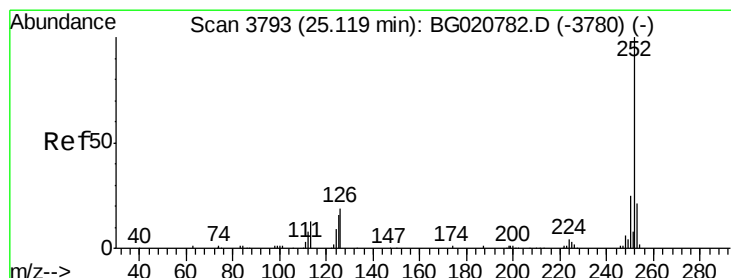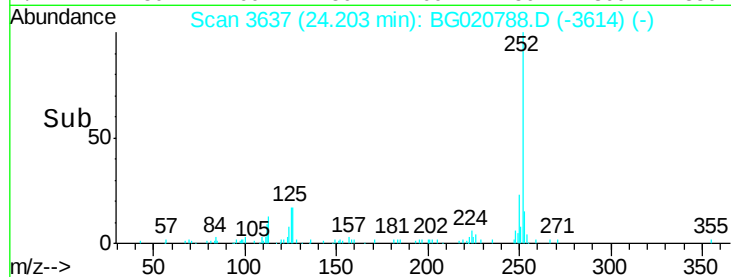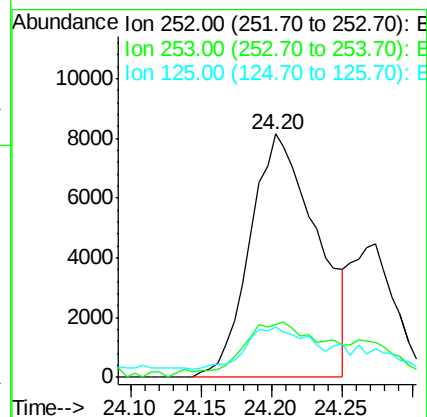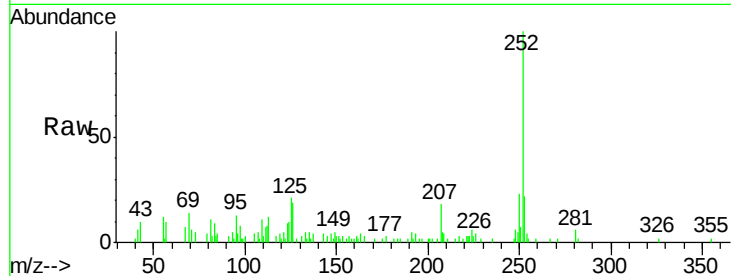

#91

Benzo(a)pyrene

Concen: 3.38 ng/ul

RT: 25.12 min Scan# 3793

Delta R.T. 0.00 min

Lab File: BG020788.D

Acq: 4 Feb 2016 15:51




Tgt Ion:252 Resp: 18636


Ion Ratio Lower Upper

252 100

253 25.5 17.2 25.8

125 22.6 5.8 8.6#

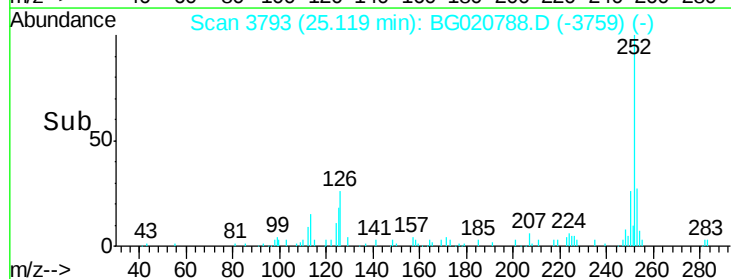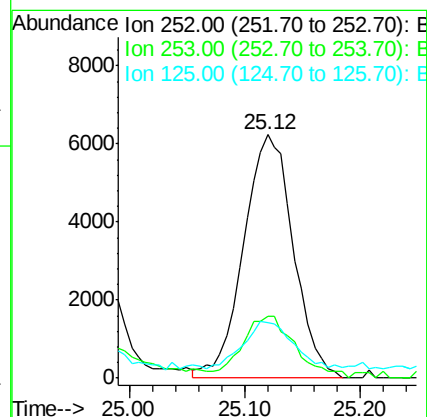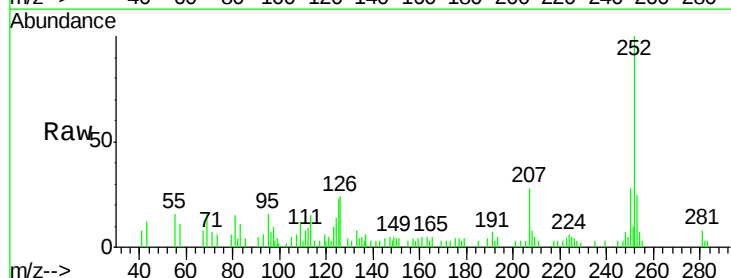

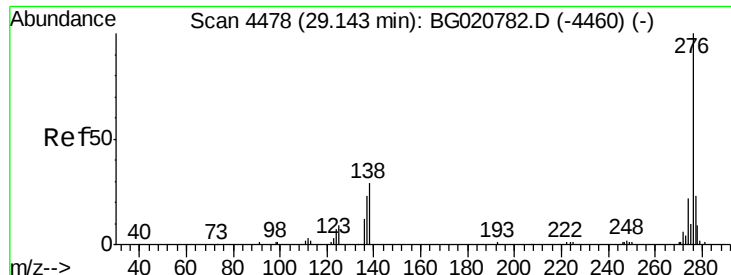

#92

Indeno(1,2,3-cd)pyrene

Concen: 2.08 ng/ul

RT: 29.14 min Scan# 4478

Delta R.T. 0.00 min

Lab File: BG020788.D


Acq: 4 Feb 2016 15:51

Instrument :

BNA_G

ClientSampleId :

BBG13

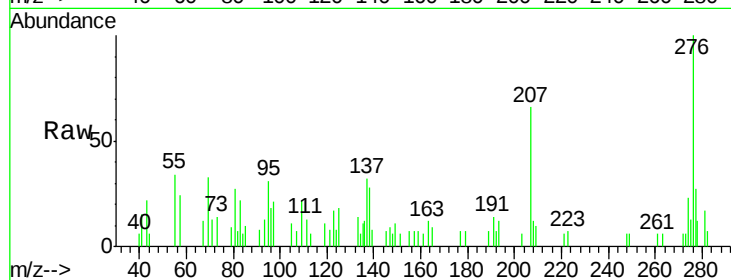


Tgt Ion:276 Resp: 13380

Ion Ratio Lower Upper

276 100

138 28.0 10.9 16.3#

277 26.5 18.9 28.3

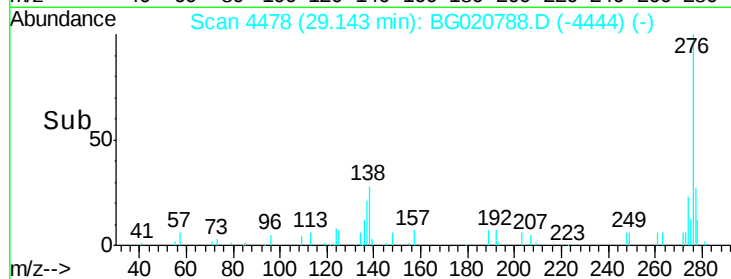

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

