

Data Path : Z:\HPCHEM1\BNA G\DATA\BG020416\
 Data File : BG020800.D
 Acq On : 5 Feb 2016 00:22
 Operator : SJ/IZ
 Sample : H1334-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BBG04

Manual Integrations
 APPROVED

mohammad
 2/5/2016 3:39:30 PM

Quant Time: Feb 05 08:02:04 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG012716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 05 07:34:32 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.28	152	21225	20.00	ng/ul	0.00
18) Naphthalene-d8	11.11	136	105892	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.89	164	59571	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.62	188	117282	20.00	ng/ul	0.00
78) Chrysene-d12	21.90	240	101780	20.00	ng/ul	0.00
86) Perylene-d12	25.28	264	95671	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.62	96	1371	3.10	ng/uL	0.00
5) Phenol-d5	7.41	99	32354	14.89	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.59	67	18474	16.32	ng/ul	0.00
9) 2-Chlorophenol-d4	7.80	132	27034	16.57	ng/ul	0.00
13) 4-Methylphenol-d8	8.97	113	28051	14.97	ng/ul	0.00
19) Nitrobenzene-d5	9.44	128	13330	20.63	ng/ul	0.00
22) 2-Nitrophenol-d4	10.17	143	12491	22.05	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.71	165	25303	16.36	ng/ul	0.00
29) 4-Chloroaniline-d4	11.23	131	39583	18.20	ng/ul	0.00
44) Dimethylphthalate-d6	14.28	166	83931	16.49	ng/ul	0.00
47) Acenaphthylene-d8	14.58	160	111557	17.99	ng/ul	0.00
52) 4-Nitrophenol-d4	15.05	143	12232	13.59	ng/ul	0.00
58) Fluorene-d10	15.87	176	73363	16.49	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.98	200	5380	13.89	ng/ul	0.00
71) Anthracene-d10	17.72	188	104085	18.05	ng/ul	0.00
79) Pyrene-d10	19.98	212	103049	18.65	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.05	264	97558	19.03	ng/ul	0.00

Target Compounds

						Ovalue
45) Dimethylphthalate	14.33	163	27431	5.16	ng/ul	99
70) Phenanthrene	17.66	178	28686	3.90	ng/ul	99
77) Fluoranthene	19.65	202	44349	5.86	ng/ul#	80
80) Pyrene	20.01	202	37420	4.86	ng/ul#	76
83) Benzo(a)anthracene	21.88	228	18068	2.76	ng/ul	95
84) Bis(2-ethylhexyl)phthalate	21.77	149	9816	2.10	ng/ul#	95
85) Chrysene	21.95	228	14359	2.36	ng/ul	98
88) Benzo(b)fluoranthene	24.21	252	19736	3.15	ng/ul#	89
89) Benzo(k)fluoranthene	24.27	252	6425	1.05	ng/ul#	92
91) Benzo(a)pyrene	25.12	252	14437	2.41	ng/ul#	87
92) Indeno(1,2,3-cd)pyrene	29.15	276	8895m	1.27	ng/ul	
94) Benzo(g,h,i)perylene	30.35	276	7795m	1.35	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG020416\
Data File : BG020800.D
Acq On : 5 Feb 2016 00:22
Operator : SJ/IZ
Sample : H1334-06
Misc :
ALS Vial : 19 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
BBG04

Manual Integrations
APPROVED

mohammad
2/5/2016 3:39:30 PM

Quant Time: Feb 05 08:02:04 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG012716.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 05 07:34:32 2016
Response via : Initial Calibration

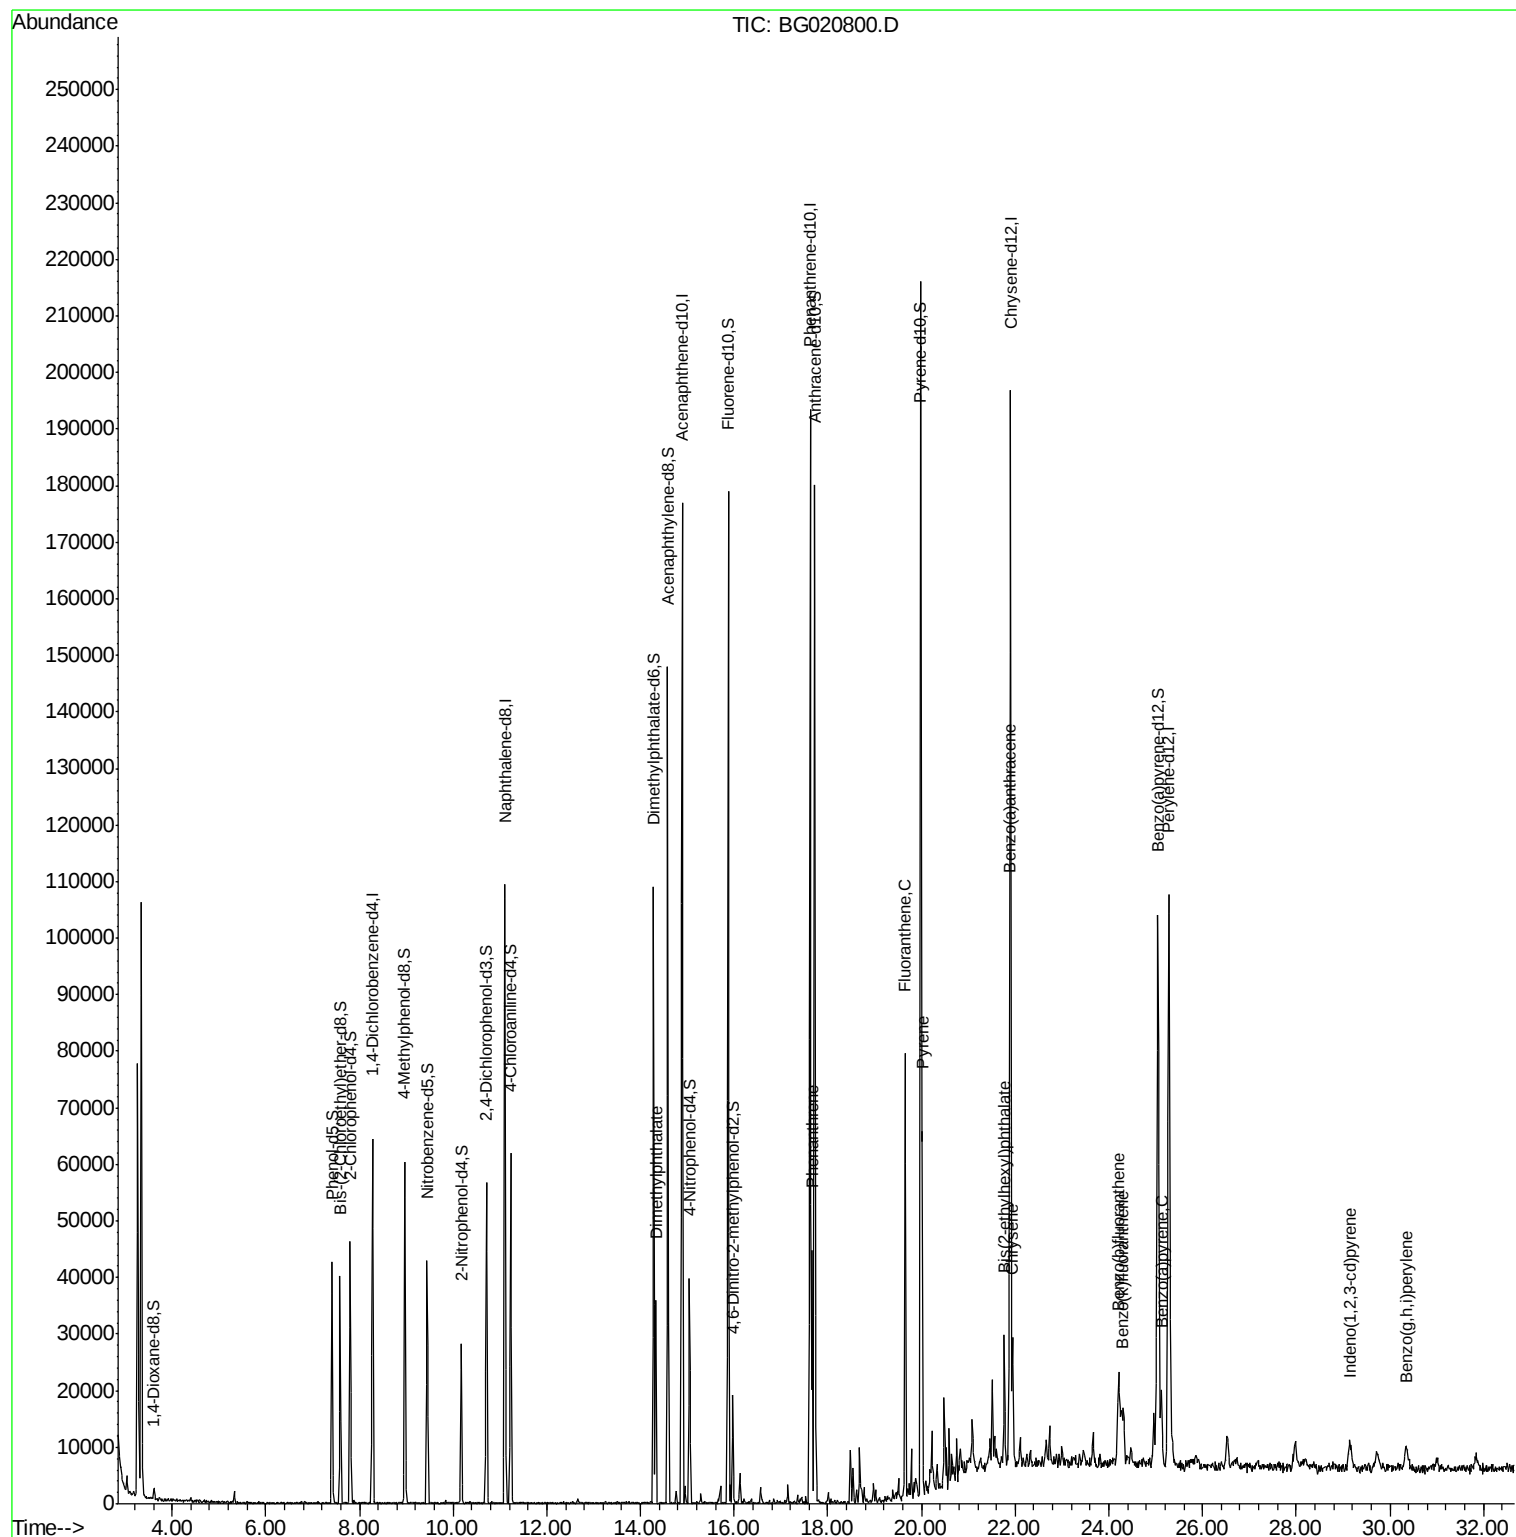

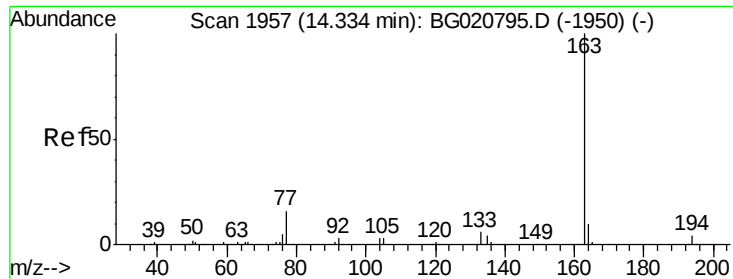





#45
 Dimethylphthalate
 Concen: 5.16 ng/ul
 RT: 14.33 min Scan# 1956
 Delta R.T. -0.00 min
 Lab File: BG020800.D
 Acq: 5 Feb 2016 00:22

Instrument :
 BNA_G
 ClientSampled :
 BBG04

Tot Ion:	163	Resp:	27431
Ion Ratio	Lower	Upper	
163	100		
194	4.7	4.0	6.0
164	10.7	8.4	12.6




Manual Integrations
 APPROVED


mohammad
 2/5/2016 3:39:30 PM

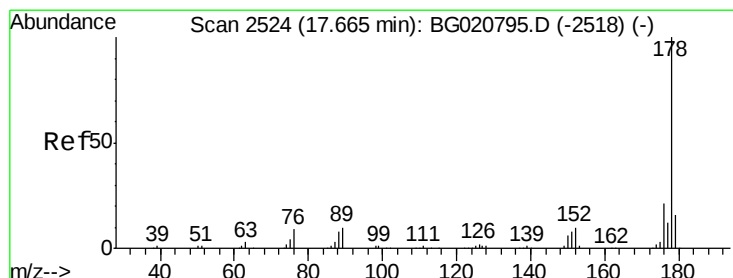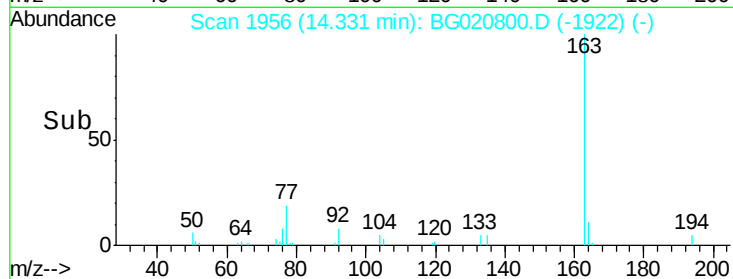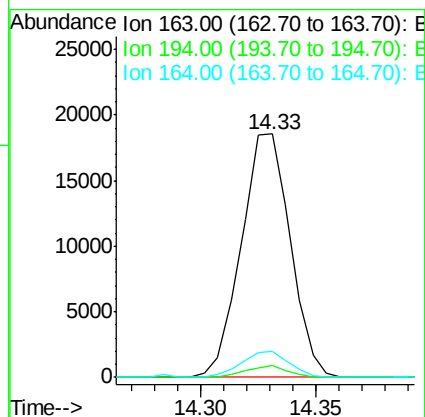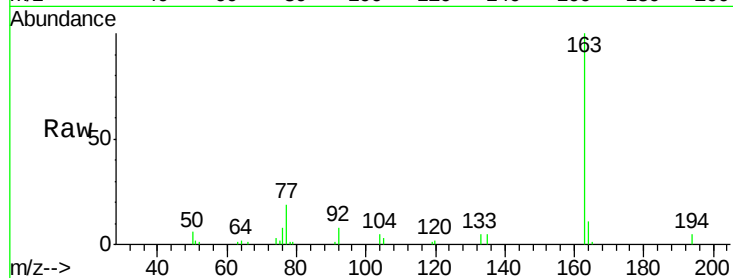

#70
 Phenanthrene
 Concen: 3.90 ng/ul
 RT: 17.66 min Scan# 2523
 Delta R.T. -0.00 min
 Lab File: BG020800.D
 Acq: 5 Feb 2016 00:22

Tgt Ion:	178	Resp:	28686
Ion Ratio	Lower	Upper	
178	100		
179	14.3	12.3	18.5
176	19.3	15.4	23.0

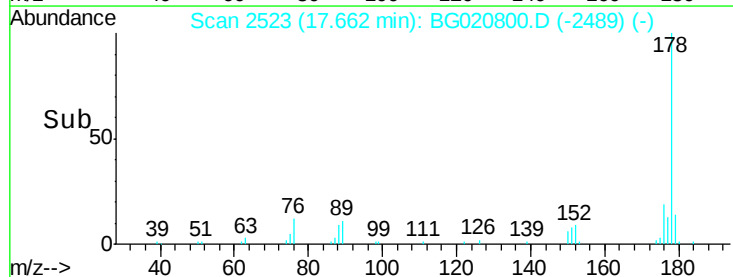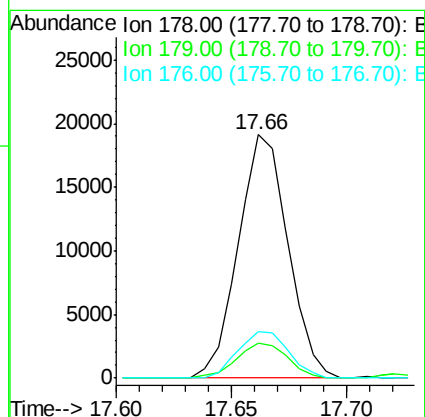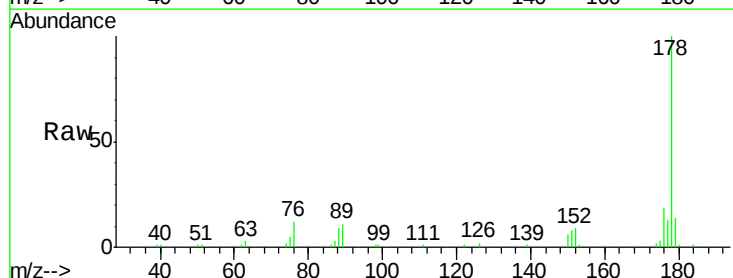

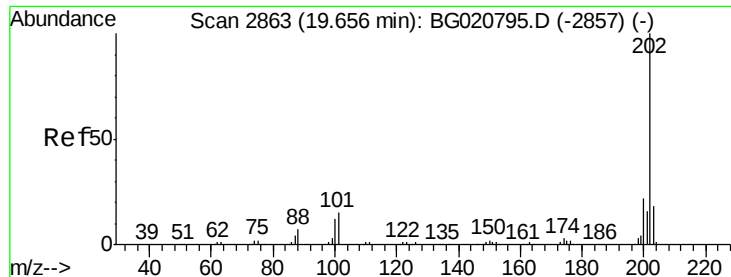

#77

Fluoranthene

Concen: 5.86 ng/ul

RT: 19.65 min Scan# 2862

Delta R.T. -0.00 min

Lab File: BG020800.D

Acq: 5 Feb 2016 00:22

Instrument :

BNA_G





ClientSampleId :

BBG04

Tot Ion:	202	Resp:	44349
Ion Ratio	Lower	Upper	
202	100		
101	15.4	6.1	9.1#
100	11.3	4.6	7.0#

Manual Integrations
APPROVED

mohammad
2/5/2016 3:39:30 PM

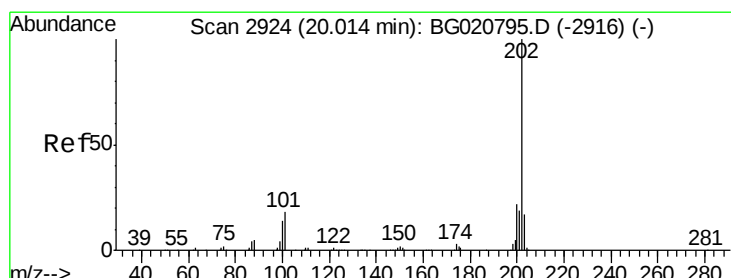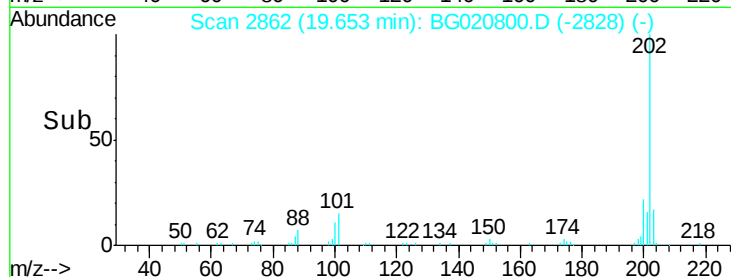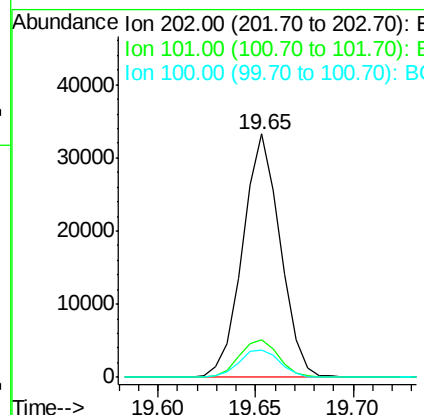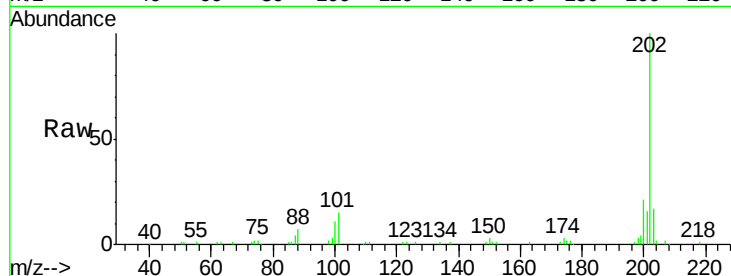

#80

Pyrene

Concen: 4.86 ng/ul




RT: 20.01 min Scan# 2923


Delta R.T. -0.00 min

Lab File: BG020800.D

Acq: 5 Feb 2016 00:22

Tgt Ion:	202	Resp:	37420
Ion Ratio	Lower	Upper	
202	100		
101	17.6	6.9	10.3#
100	15.1	5.6	8.4#

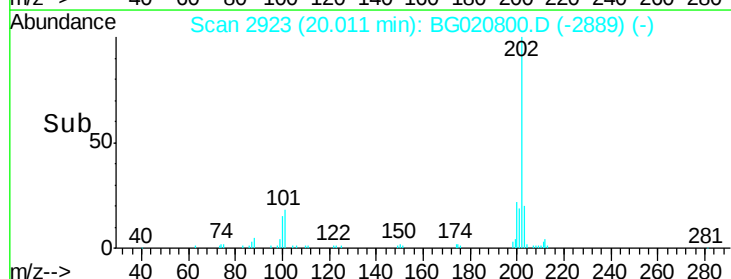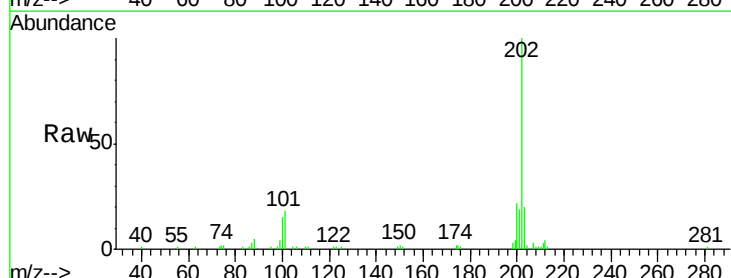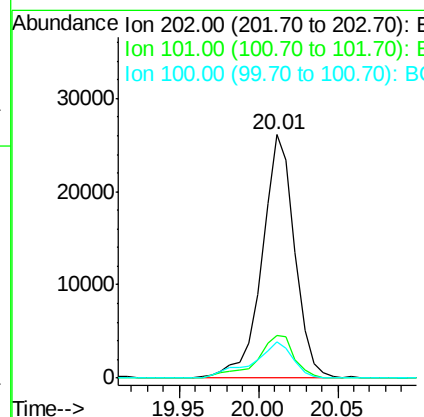

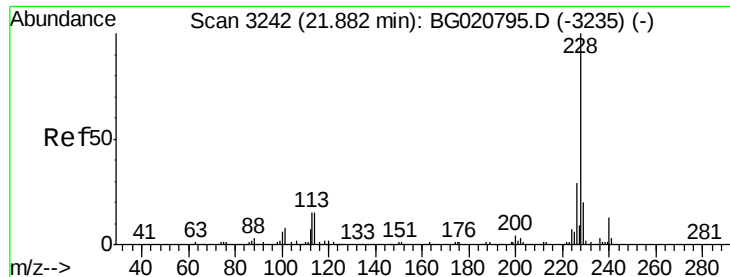

#83

Benzo(a)anthracene

Concen: 2.76 ng/ul

RT: 21.88 min Scan# 3241

Delta R.T. -0.00 min

Lab File: BG020800.D

Acq: 5 Feb 2016 00:22

Instrument :

BNA_G


ClientSampled :

BBG04




Tot Ion:	228	Resp:	18068
Ion Ratio	Lower	Upper	
228	100		
229	22.3	16.0	24.0
226	30.3	21.8	32.8

Manual Integrations
APPROVED

mohammad
2/5/2016 3:39:30 PM

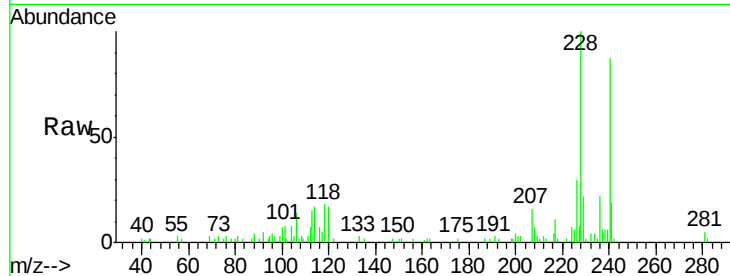

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 229.00 (228.70 to 229.70): E
Ion 226.00 (225.70 to 226.70): E

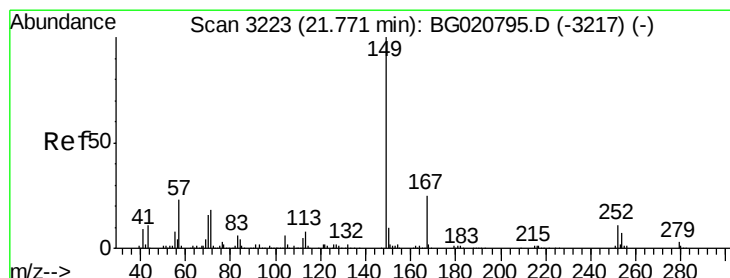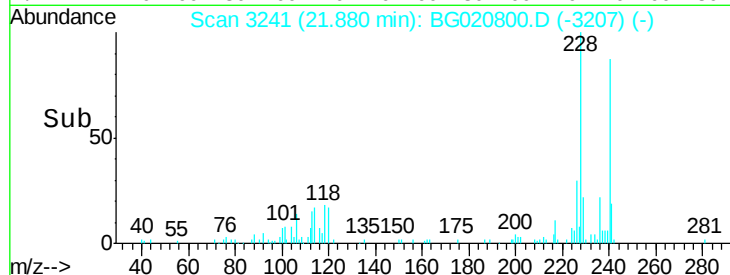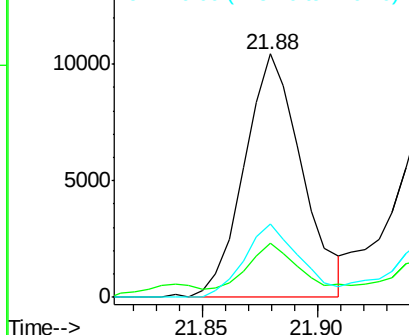

#84

Bis(2-ethylhexyl)phthalate

Concen: 2.10 ng/ul


RT: 21.77 min Scan# 3222

Delta R.T. -0.00 min



Lab File: BG020800.D


Acq: 5 Feb 2016 00:22

Tgt Ion:	149	Resp:	9816
Ion Ratio	Lower	Upper	
149	100		
167	26.4	23.0	34.6
279	2.6	4.3	6.5#

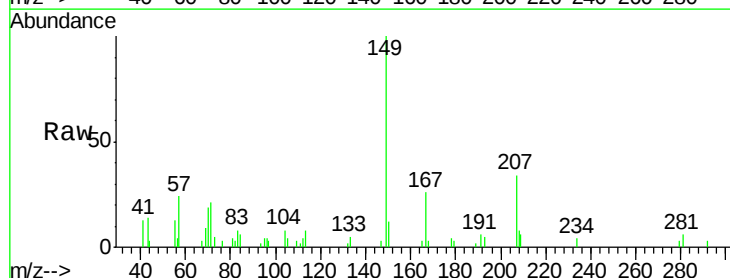

Abundance Ion 149.00 (148.70 to 149.70): E
Ion 167.00 (166.70 to 167.70): E
Ion 279.00 (278.70 to 279.70): E

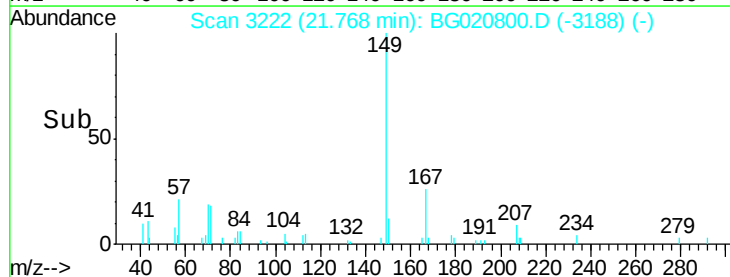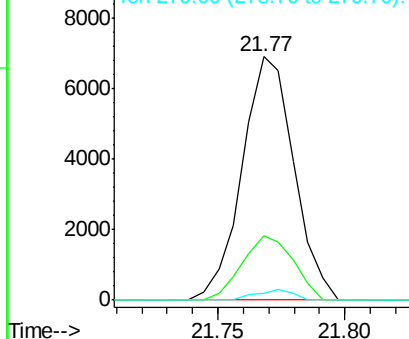

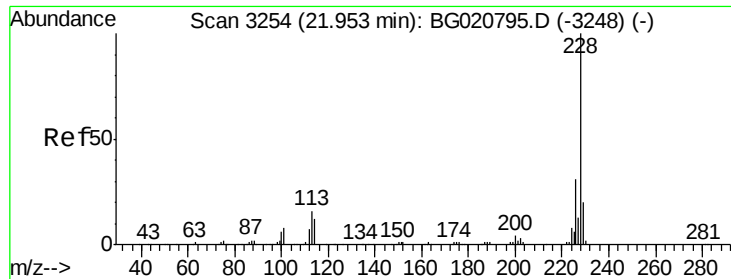

#85
Chrysene
Concen: 2.36 ng/ul
RT: 21.95 min Scan# 3253
Delta R.T. -0.00 min
Lab File: BG020800.D
Acq: 5 Feb 2016 00:22

Instrument :
BNA_G
ClientSampleId :
BBG04




Tot Ion:228	Resp:	14359
Ion Ratio	Lower	Upper
228	100	
226	31.1	24.1 36.1
229	21.1	16.0 24.0

Manual Integrations
APPROVED

mohammad
2/5/2016 3:39:30 PM




Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

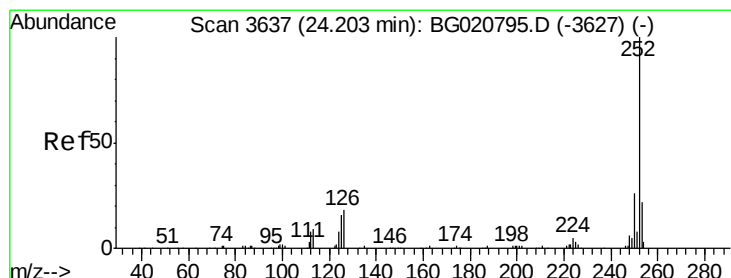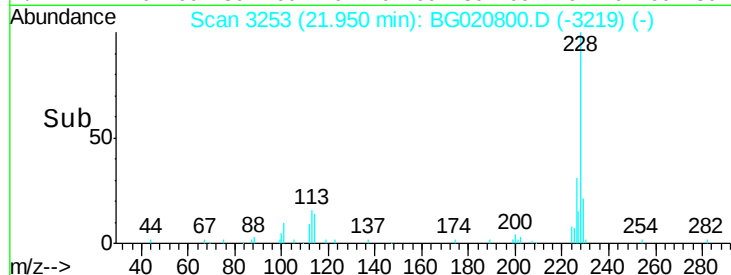
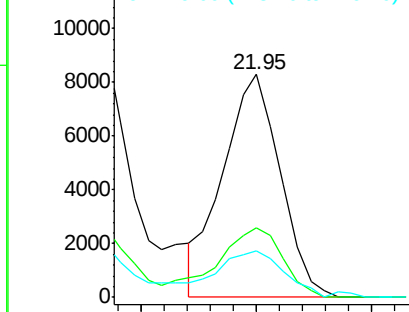



#88
Benzo(b)fluoranthene
Concen: 3.15 ng/ul
RT: 24.21 min Scan# 3637
Delta R.T. 0.00 min
Lab File: BG020800.D
Acq: 5 Feb 2016 00:22

Tgt Ion:252	Resp:	19736
Ion Ratio	Lower	Upper
252	100	
253	23.3	17.4 26.0
125	18.7	4.9 7.3#

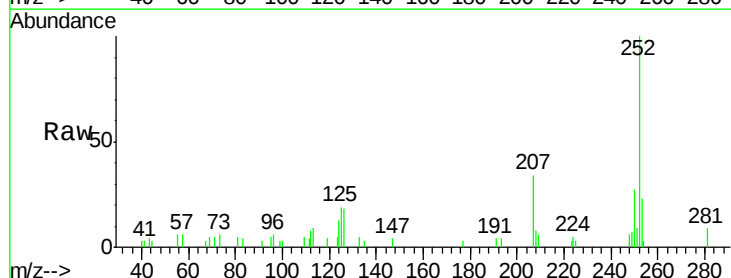

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

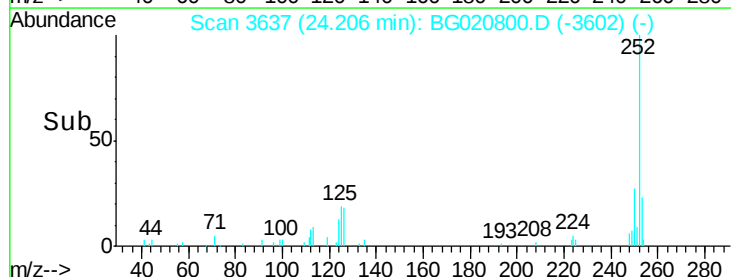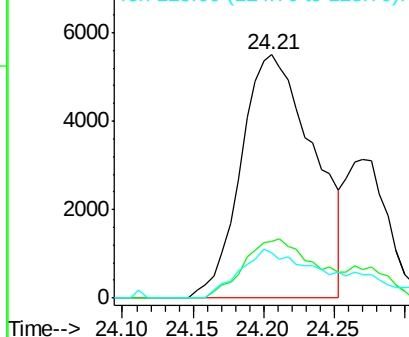

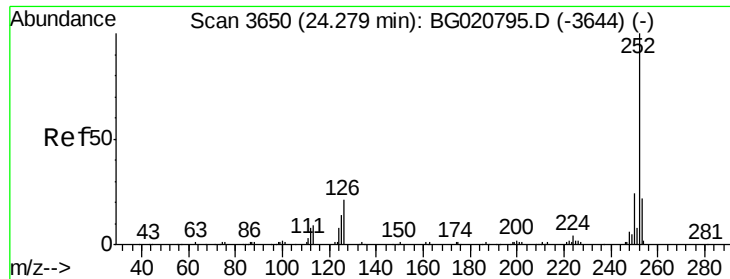





#89
Benzo(k)fluoranthene
Concen: 1.05 ng/ul
RT: 24.27 min Scan# 3648
Delta R.T. -0.01 min
Lab File: BG020800.D
Acq: 5 Feb 2016 00:22

Instrument :
BNA_G
ClientSampleId :
BBG04

Tot Ion	Ratio	Lower	Upper
252	100		
253	20.9	17.1	25.7
125	17.0	5.4	8.0#




Manual Integrations
APPROVED


mohammad
2/5/2016 3:39:30 PM

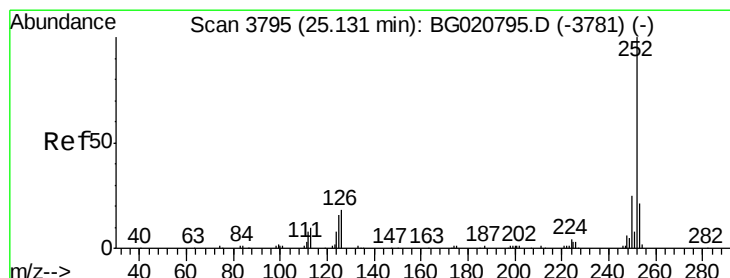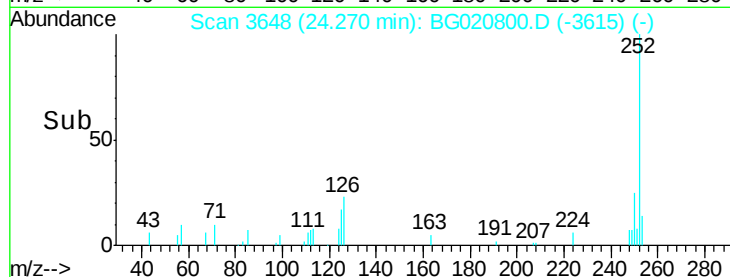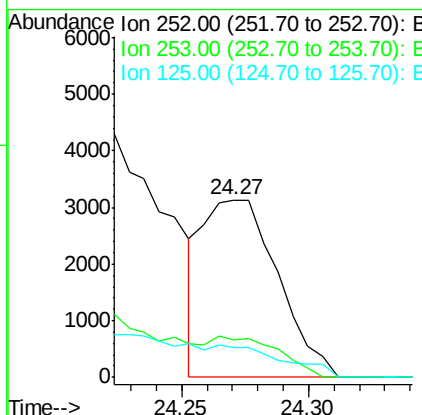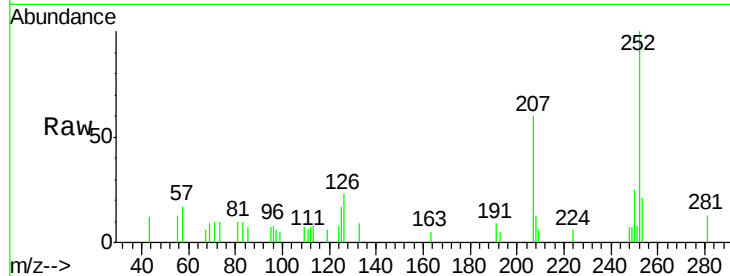

#91
Benzo(a)pyrene
Concen: 2.41 ng/ul
RT: 25.12 min Scan# 3793
Delta R.T. -0.01 min
Lab File: BG020800.D
Acq: 5 Feb 2016 00:22

Tgt Ion	Ratio	Lower	Upper
252	100		
253	25.6	17.2	25.8
125	16.5	5.8	8.6#

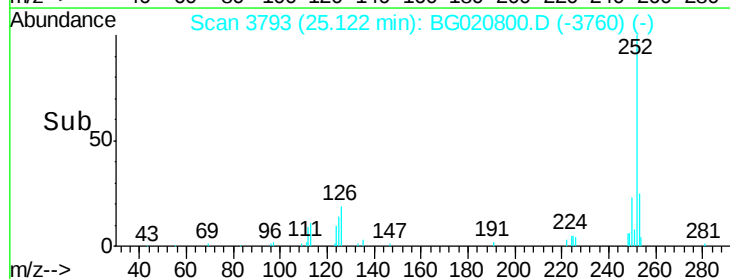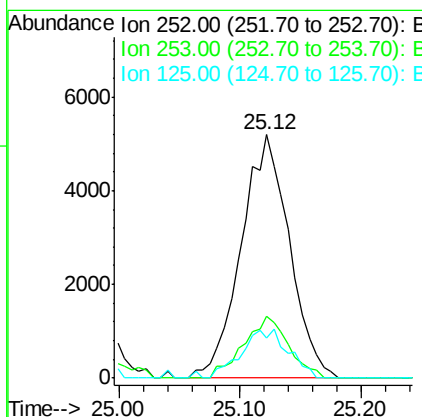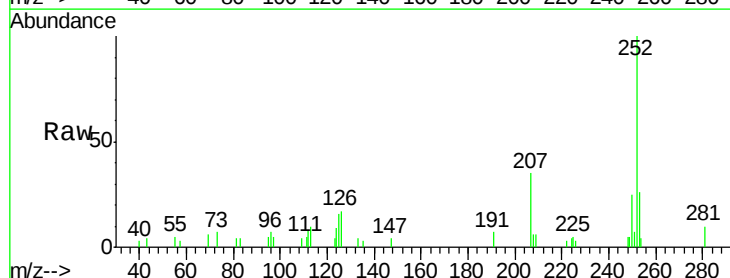

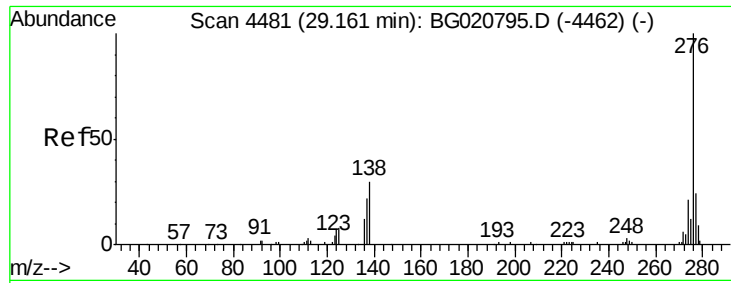

#92


Indeno(1,2,3-cd)pyrene
Concen: 1.27 ng/ul m
RT: 29.15 min Scan# 4479
Delta R.T. -0.01 min
Lab File: BG020800.D
Acq: 5 Feb 2016 00:22

Instrument :
BNA_G
ClientSampleId :
BBG04




Tot Ion	Ratio	Lower	Upper
276	100		
138	29.7	10.9	16.3#
277	24.3	18.9	28.3

Manual Integrations
APPROVED

mohammad
2/5/2016 3:39:30 PM

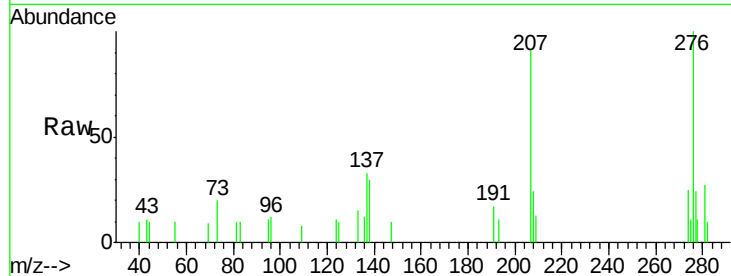


Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 277.00 (276.70 to 277.70): E

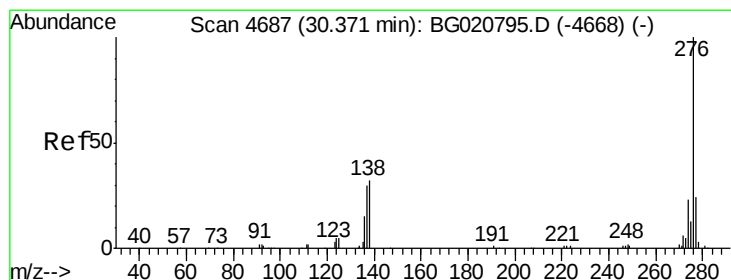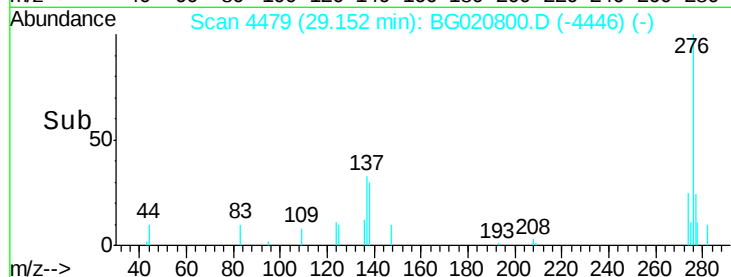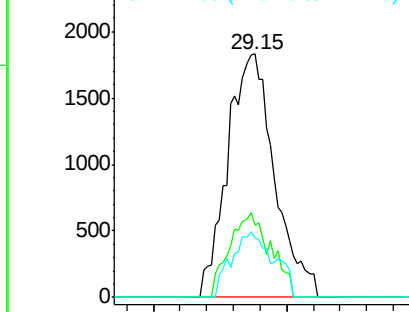

#94

Benzo(g,h,i)perylene
Concen: 1.35 ng/ul m
RT: 30.35 min Scan# 4683
Delta R.T. -0.02 min
Lab File: BG020800.D
Acq: 5 Feb 2016 00:22

Tgt Ion	Ratio	Lower	Upper
276	100		
138	25.5	11.2	16.8#
277	25.2	19.0	28.6

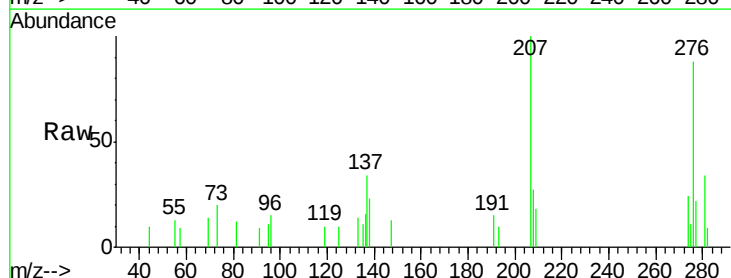

Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 277.00 (276.70 to 277.70): E

