


Data Path : Z:\HPCHEM1\BNA_G\Data\BG020417\
 Data File : BG025797.D
 Acq On : 3 Feb 2017 16:31
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG013017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 30 18:29:38 2017

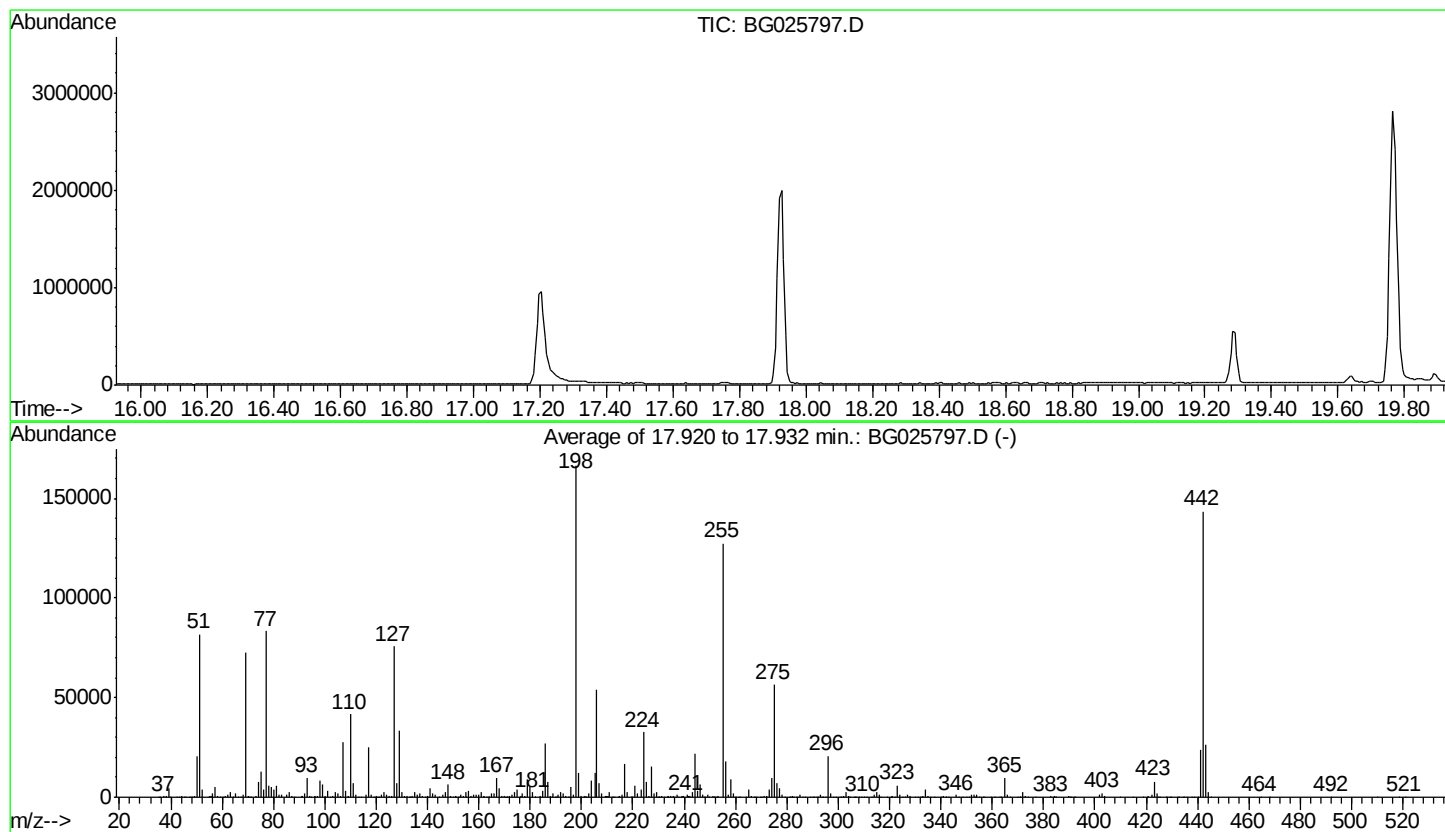

AutoFind: Scans 2567, 2568, 2569; Background Corrected with Scan 2559

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.2	81920	PASS
68	69	0.00	2	1.5	1119	PASS
69	198	0.00	100	43.8	72842	PASS
70	69	0.00	2	0.6	412	PASS
127	198	10	80	45.4	75608	PASS
197	198	0.00	2	0.7	1223	PASS
198	198	100	100	100.0	166410	PASS
199	198	5	9	7.3	12118	PASS
275	198	10	60	34.0	56520	PASS
365	198	1	100	5.8	9651	PASS
441	442	0.01	24	16.6	23786	PASS
442	198	50	100	86.2	143522	PASS
443	442	15	24	18.4	26397	PASS