
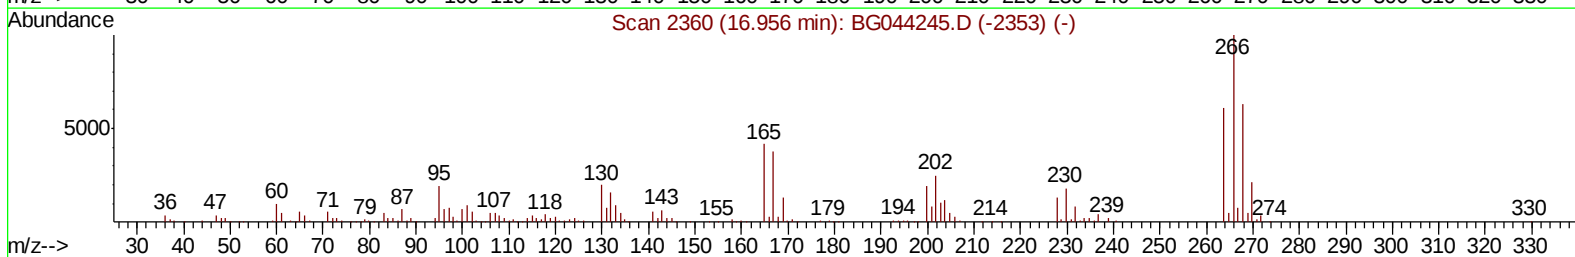
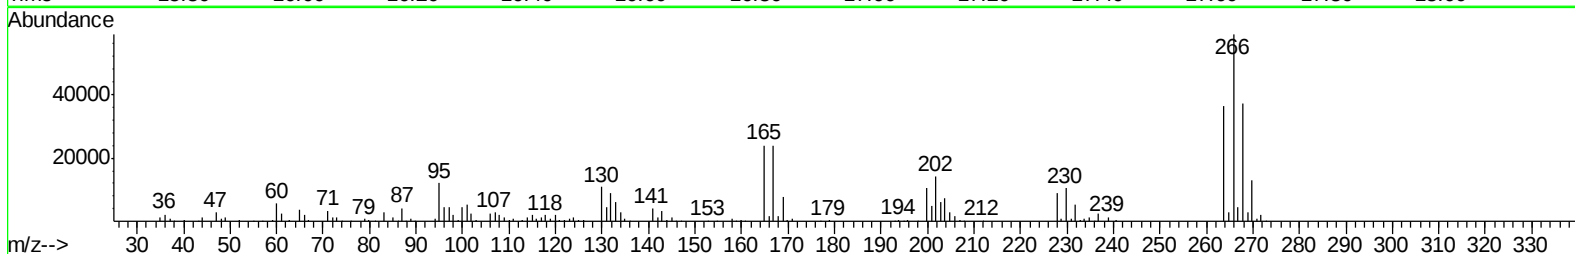


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG020420\
Data File : BG044281.D
Acq On : 4 Feb 2020 14:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 05 05:51:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG013020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 30 16:05:09 2020
Response via : Initial Calibration

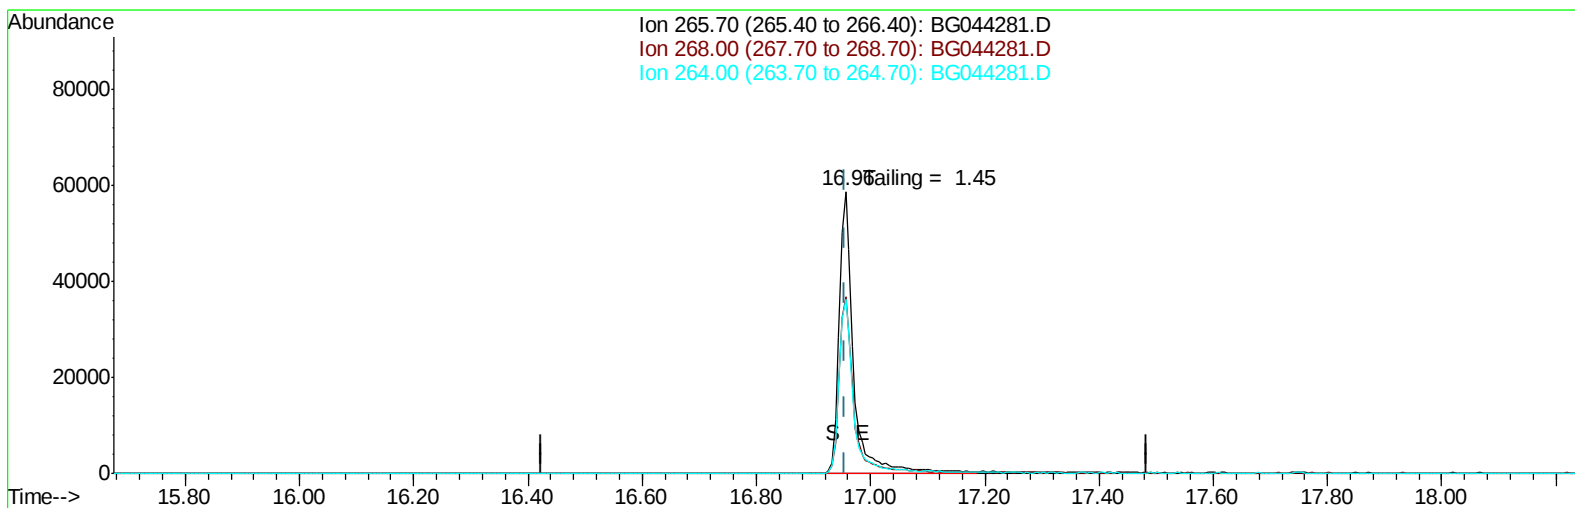

TIC: BG044281.D

(70) Pentachlorophenol (C)




16.956min (+0.001) 31139.45ng

response 102421

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	62.80
264.00	60.90	61.91
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG020420\
 Data File : BG044281.D
 Acq On : 4 Feb 2020 14:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 05 05:51:38 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG013020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 30 16:05:09 2020
 Response via : Initial Calibration

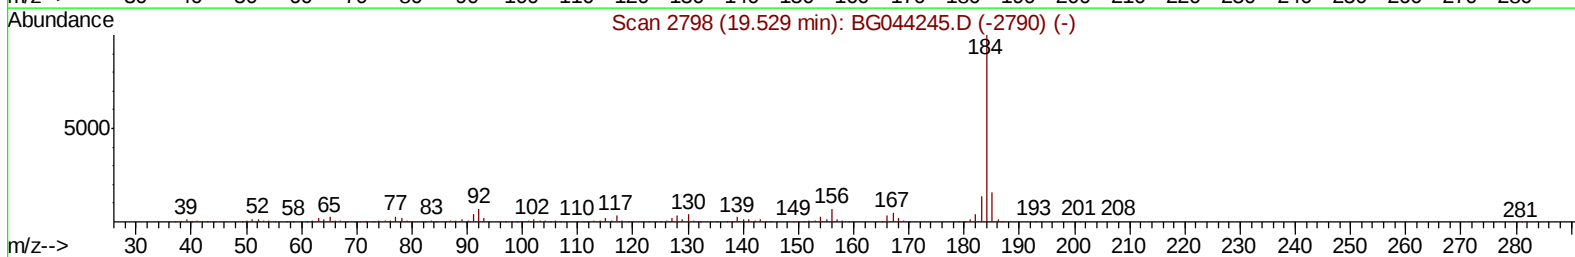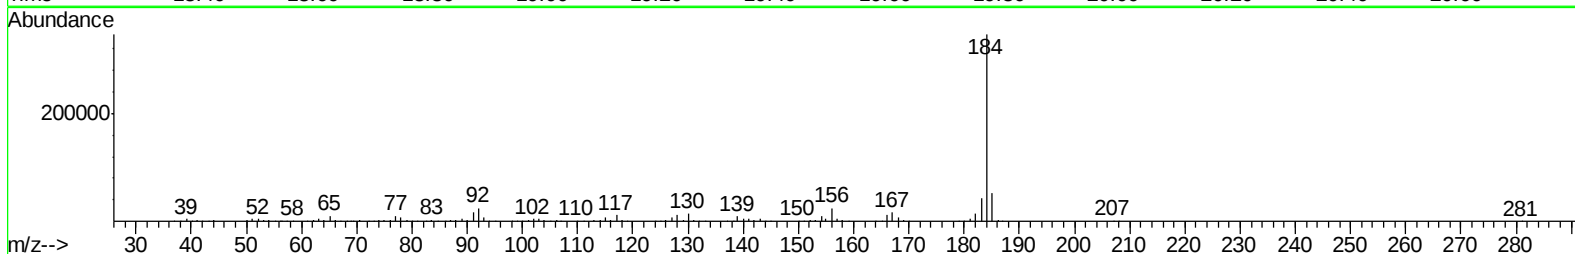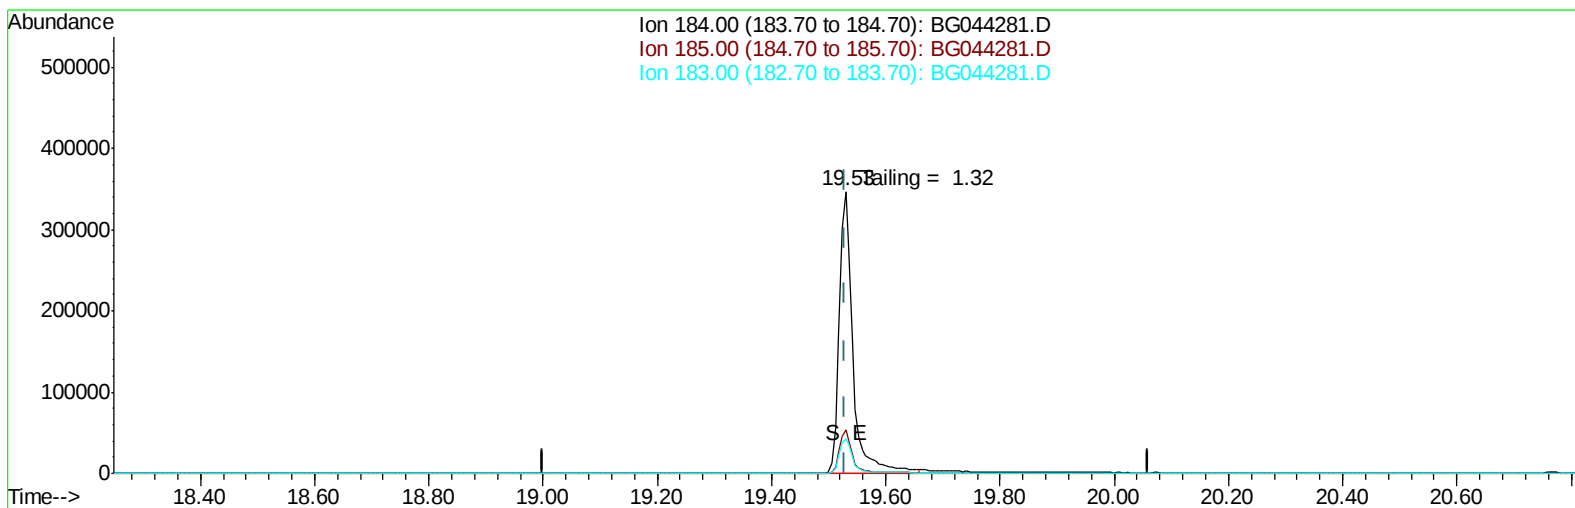

TIC: BG044281.D

(77) Benzidine

19.529min (-0.000) 0.00ng

response 600903

Ion	Exp%	Act%
184.00	100	100
185.00	16.10	15.28
183.00	13.50	12.51
0.00	0.00	0.00