
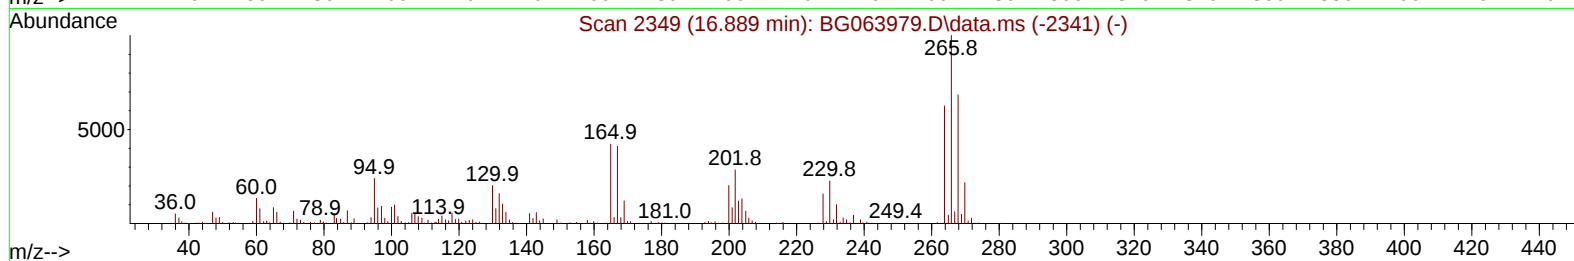
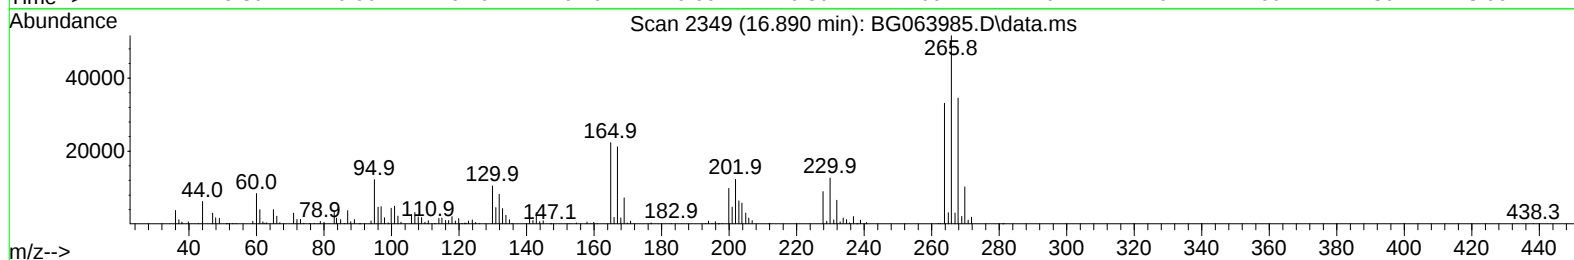


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020425\
Data File : BG063985.D
Acq On : 4 Feb 2025 9:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 11:48:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 04 02:51:00 2025
Response via : Initial Calibration

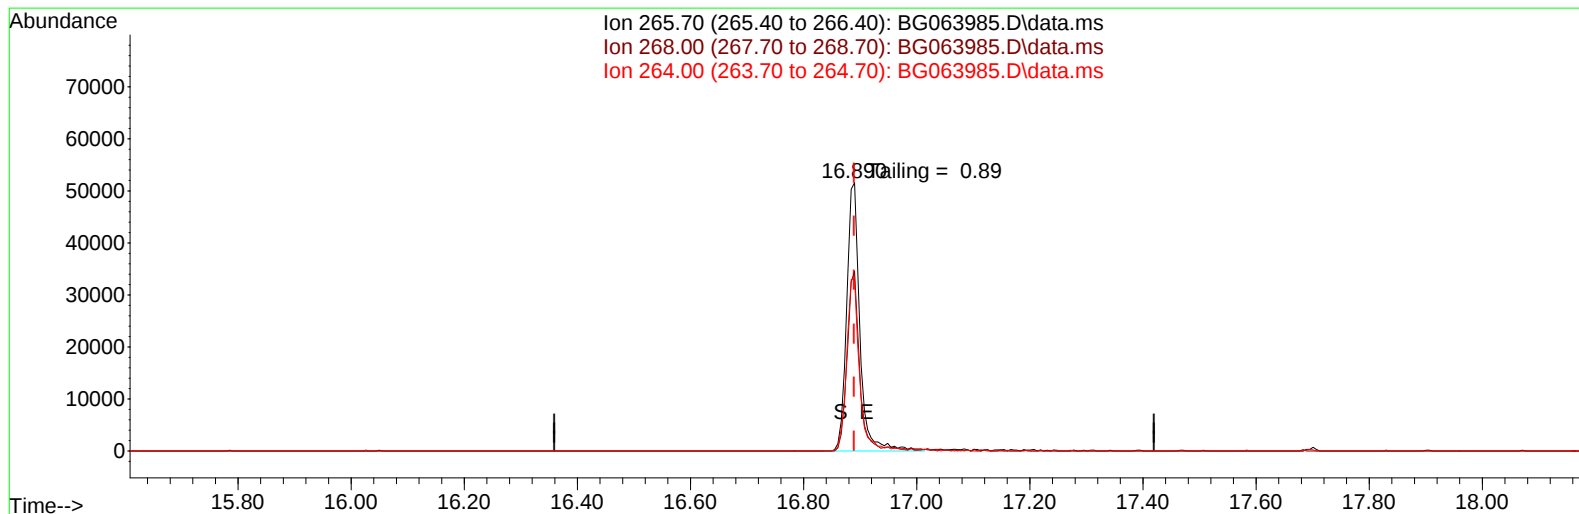

TIC: BG063985.D\data.ms

(70) Pentachlorophenol (C)




16.890min (+ 0.001) 11188.44 ng

response 84001

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.50	66.89
264.00	62.50	64.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020425\
Data File : BG063985.D
Acq On : 4 Feb 2025 9:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 04 11:48:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 04 02:51:00 2025
Response via : Initial Calibration

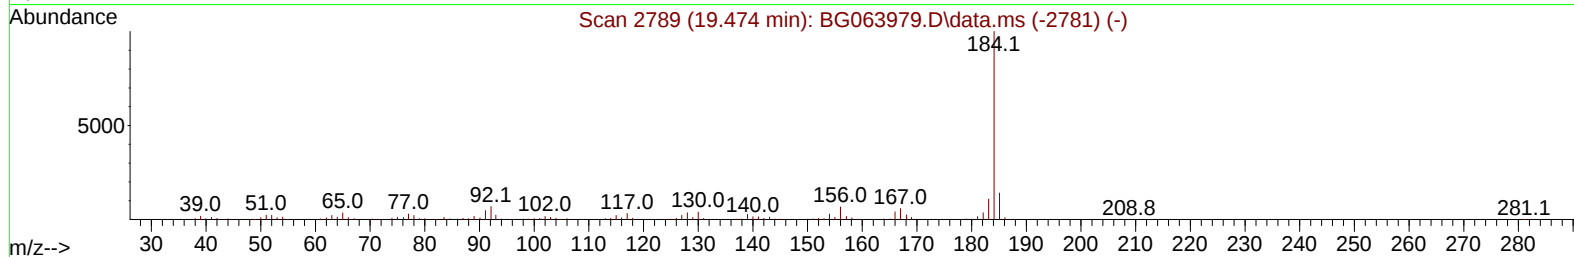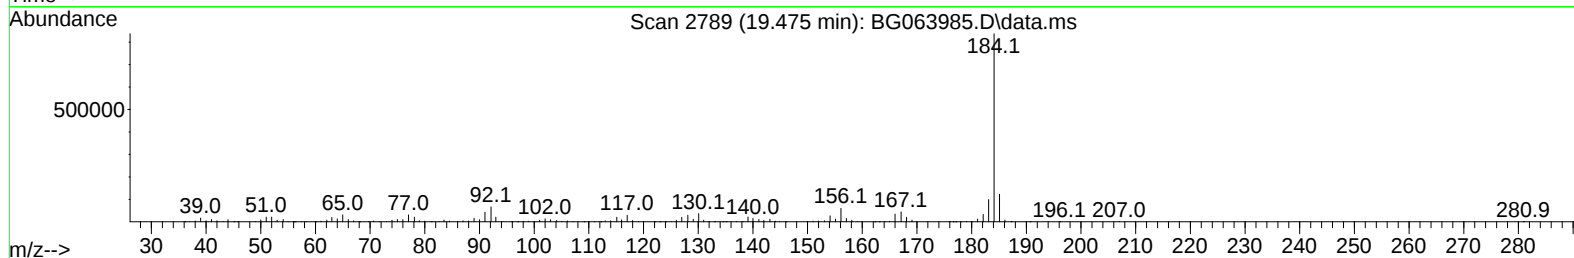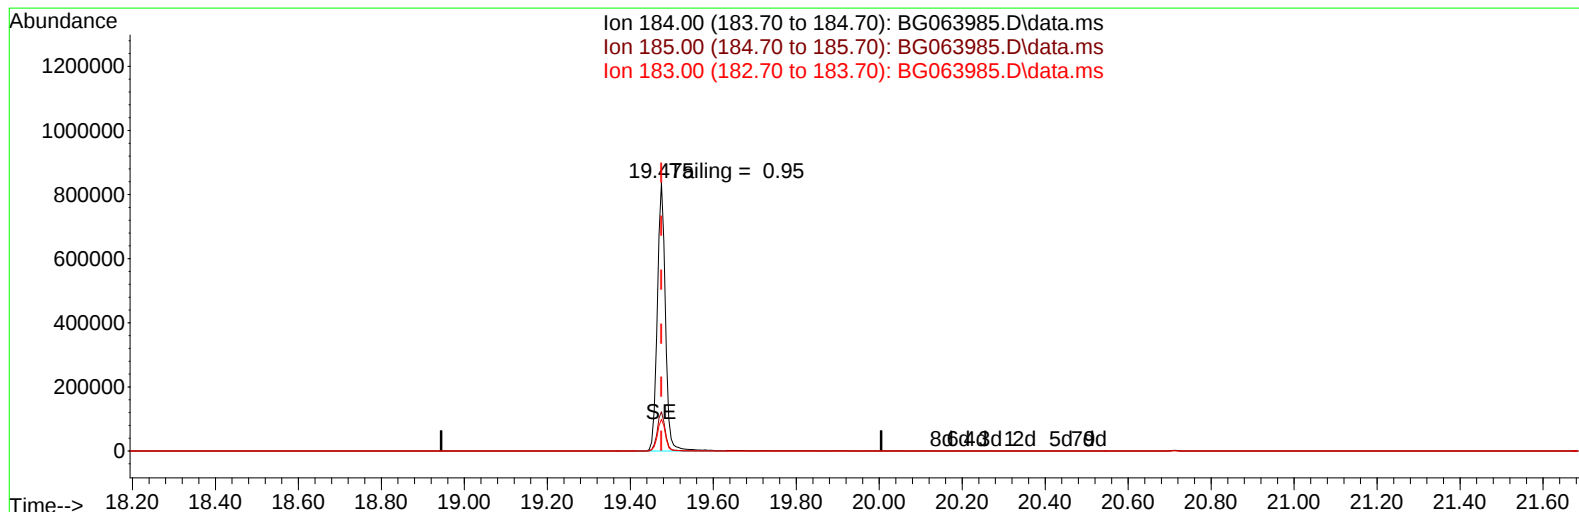

TIC: BG063985.D\data.ms

(77) Benzidine

19.475min (+ 0.001) 996271.62 ng m

response 1166821

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.64
183.00	10.90	11.81
0.00	0.00	0.00