
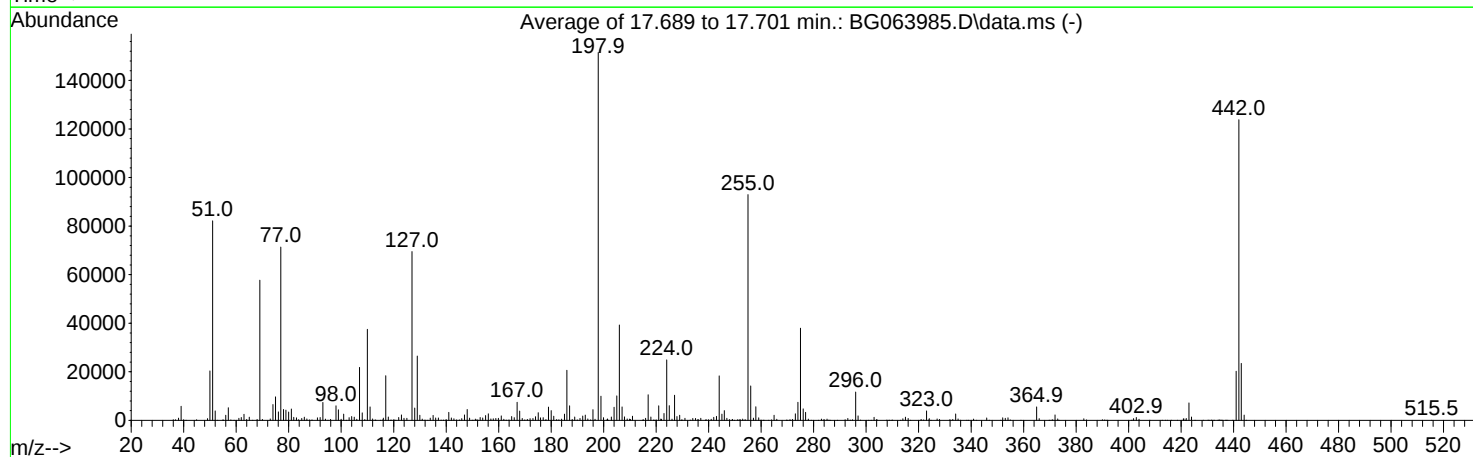


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020425\
Data File : BG063985.D
Acq On : 4 Feb 2025 9:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Feb 04 02:51:00 2025

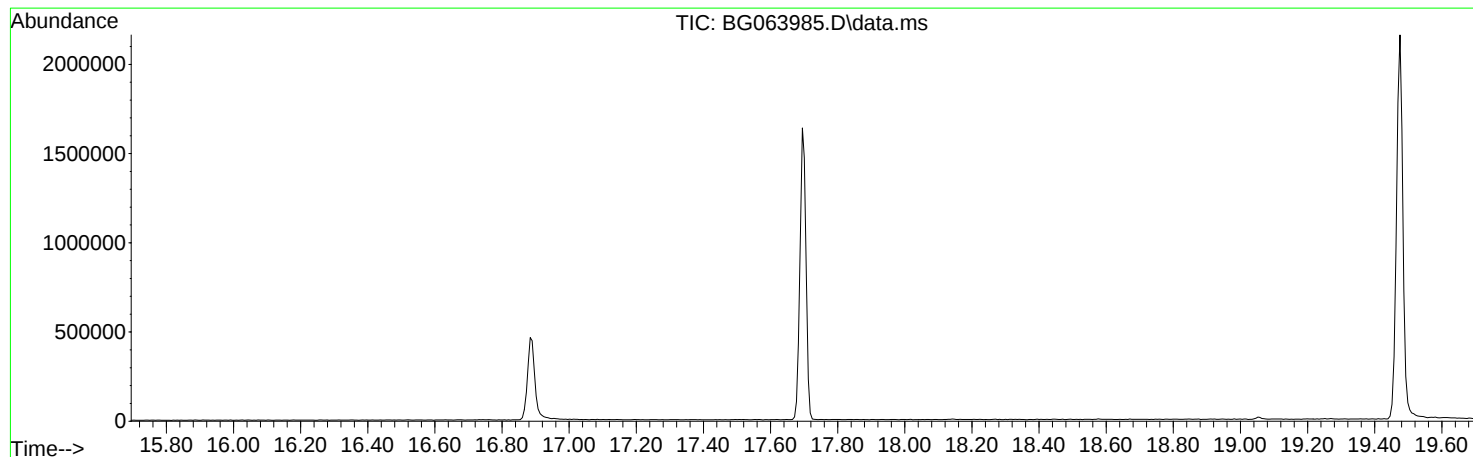

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.2	82163	PASS
68	69	0.00	2	0.7	414	PASS
69	198	0.00	100	38.1	57749	PASS
70	69	0.00	2	0.7	385	PASS
127	198	10	80	45.9	69501	PASS
197	198	0.00	2	0.3	481	PASS
198	198	100	100	100.0	151483	PASS
199	198	5	9	6.6	9957	PASS
275	198	10	60	25.1	37960	PASS
365	198	1	100	3.6	5519	PASS
441	198	0.01	100	13.3	20207	PASS
442	442	50	100	100.0	123835	PASS
443	442	15	24	18.9	23438	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/4/2025	BNA_G	<u>BG063985.D</u>
Compound Name	Response	Retention Time
DDT	328968	20.715
DDD	7983	20.274
DDE	112	19.786
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8095	337063	2.40

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020425\
Data File : BG063985.D
Acq On : 4 Feb 2025 9:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 04 11:48:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 04 02:51:00 2025
Response via : Initial Calibration

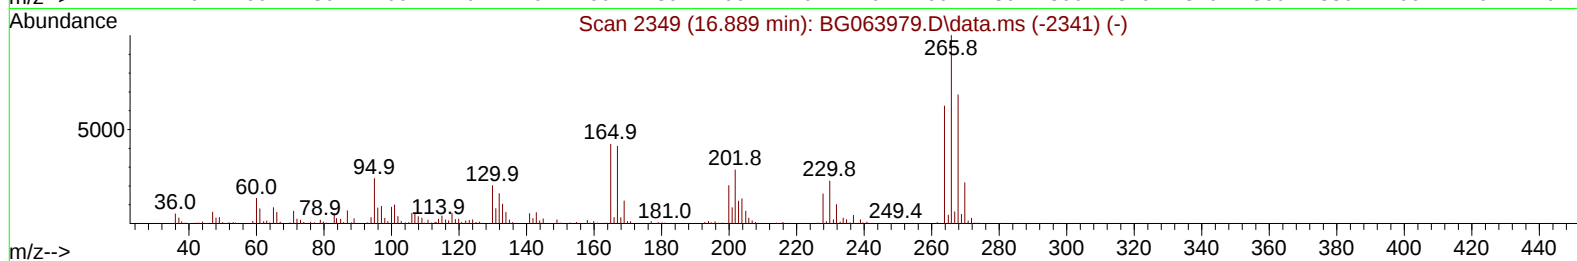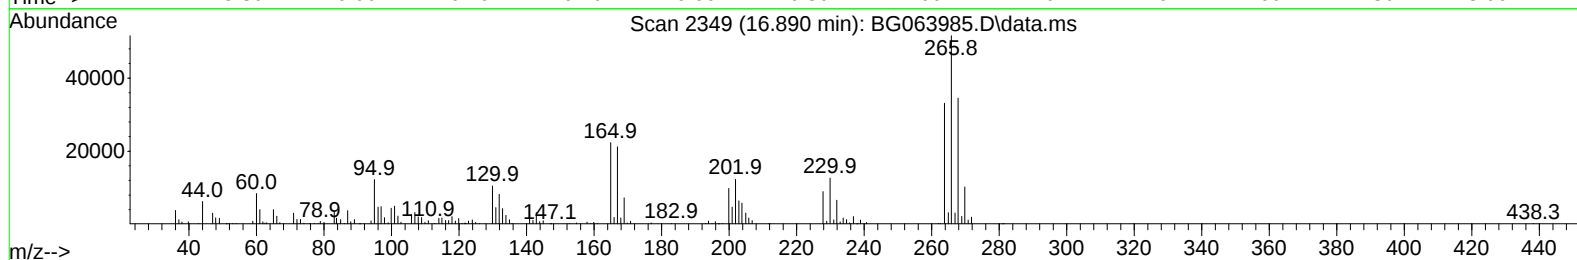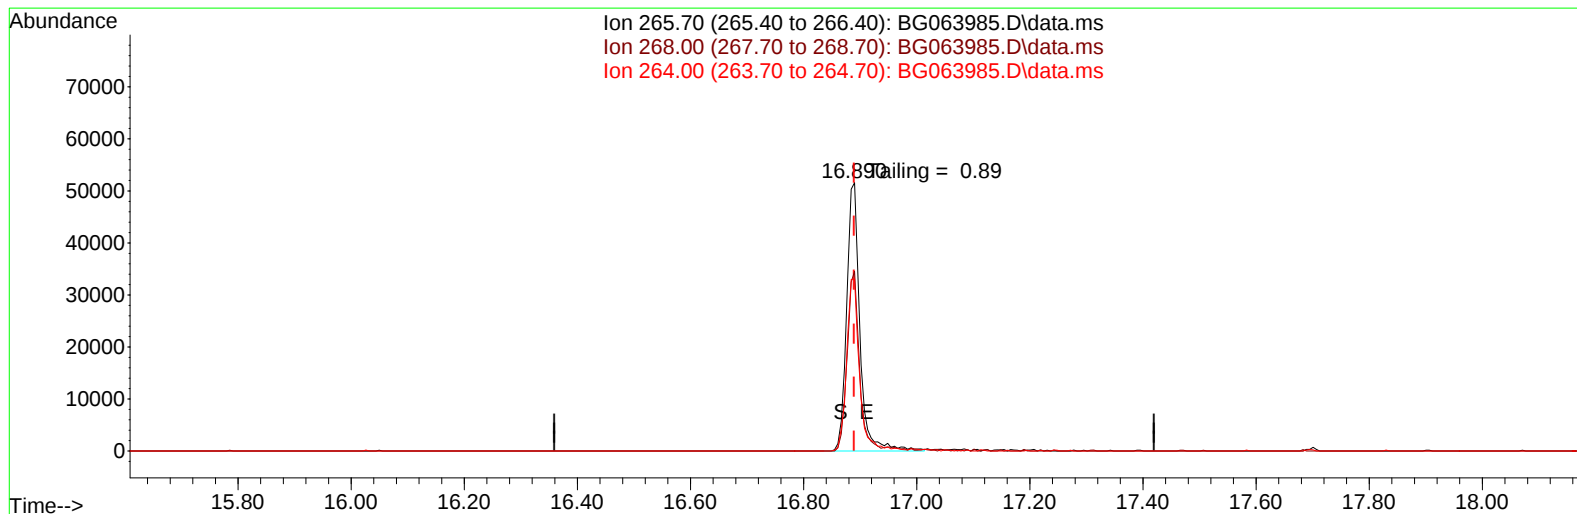

TIC: BG063985.D\data.ms

(70) Pentachlorophenol (C)

16.890min (+ 0.001) 11188.44 ng




response 84001

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.50	66.89
264.00	62.50	64.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020425\
Data File : BG063985.D
Acq On : 4 Feb 2025 9:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 04 11:48:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 04 02:51:00 2025
Response via : Initial Calibration

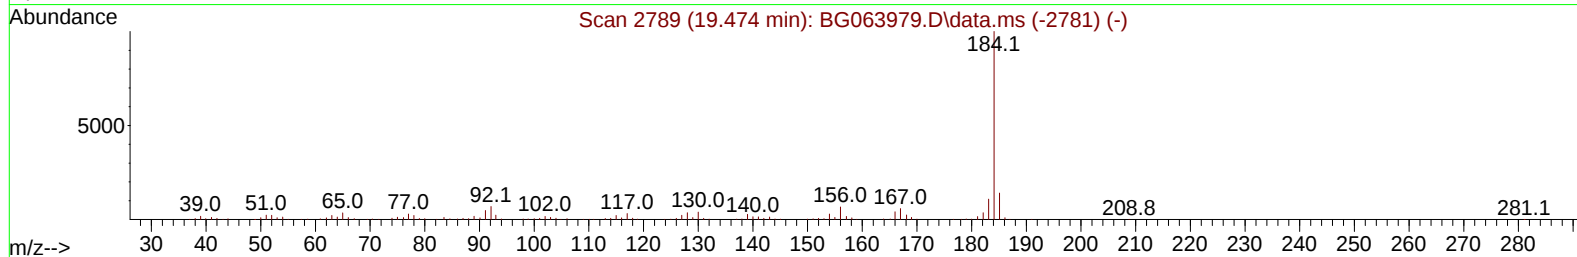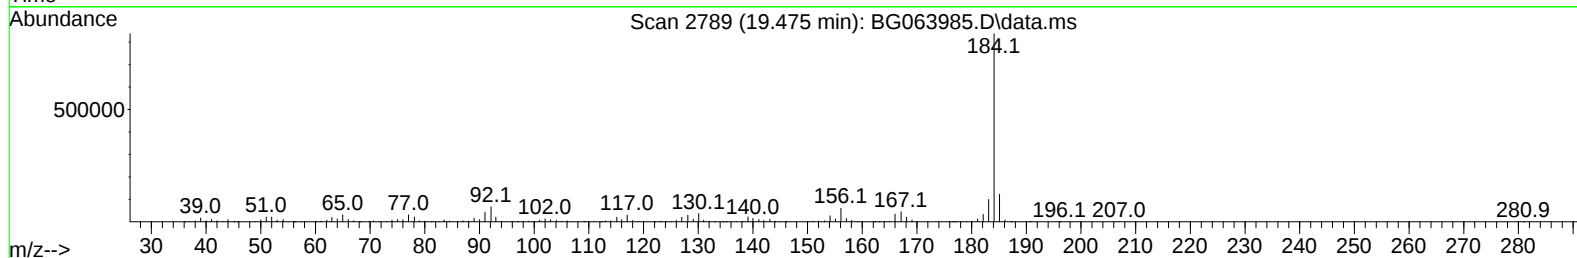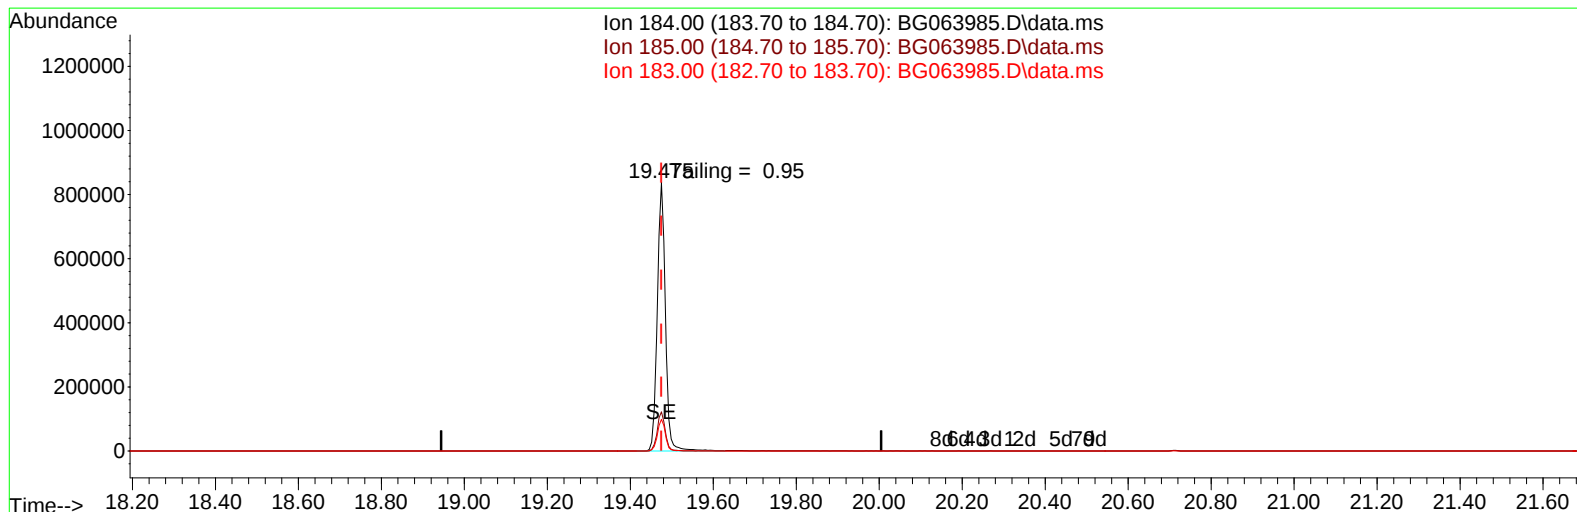

TIC: BG063985.D\data.ms

(77) Benzidine

19.475min (+ 0.001) 996271.62 ng m

response 1166821

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.64
183.00	10.90	11.81
0.00	0.00	0.00