
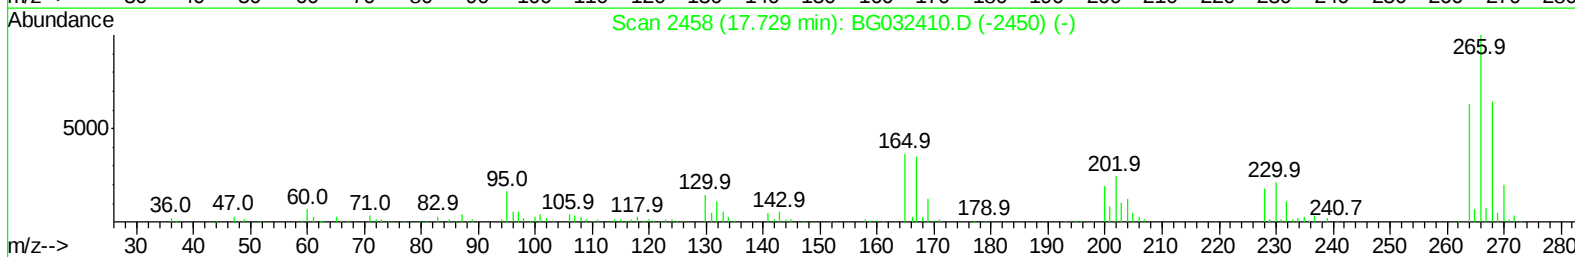
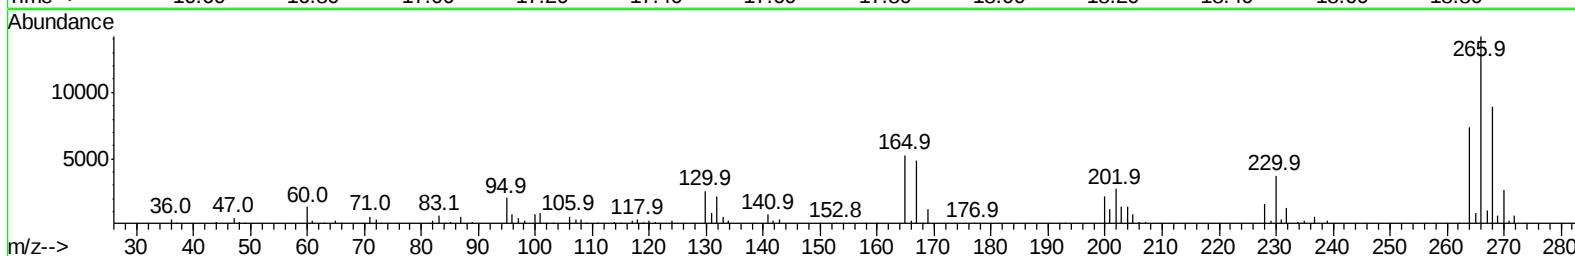


Data Path : U:\HPCHEM1\BNA G\DATA\BG020518\
Data File : BG032534.D
Acq On : 5 Feb 2018 15:15
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 08:34:39 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 29 15:32:55 2018
Response via : Initial Calibration

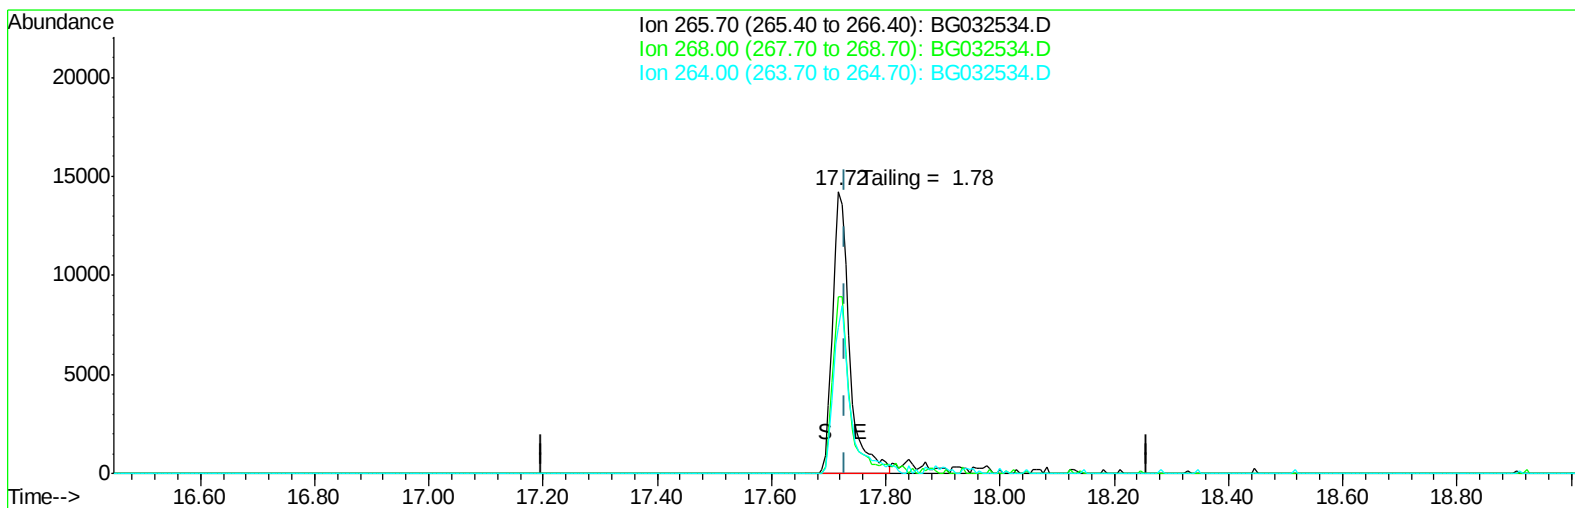

TIC: BG032534.D

(69) Pentachlorophenol (C)




17.717min (-0.011) 52799.96ng

response 29283

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.84
264.00	62.00	52.00
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA G\DATA\BG020518\
Data File : BG032534.D
Acq On : 5 Feb 2018 15:15
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 08:34:39 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 29 15:32:55 2018
Response via : Initial Calibration

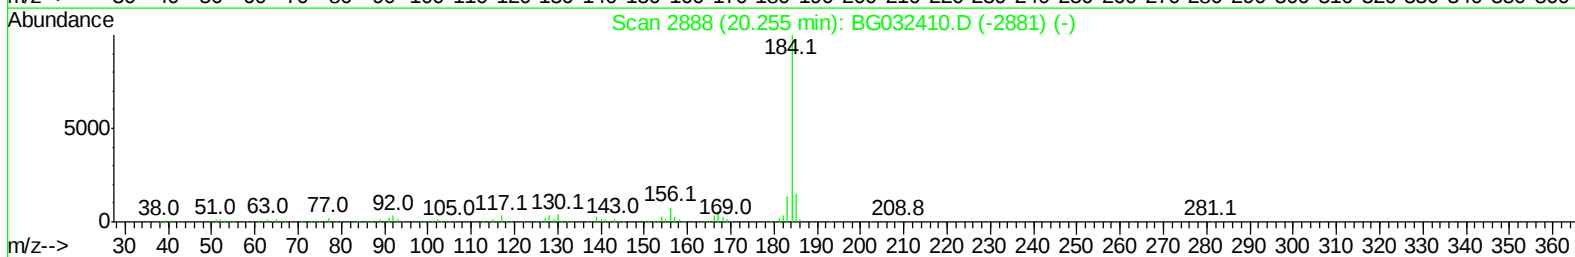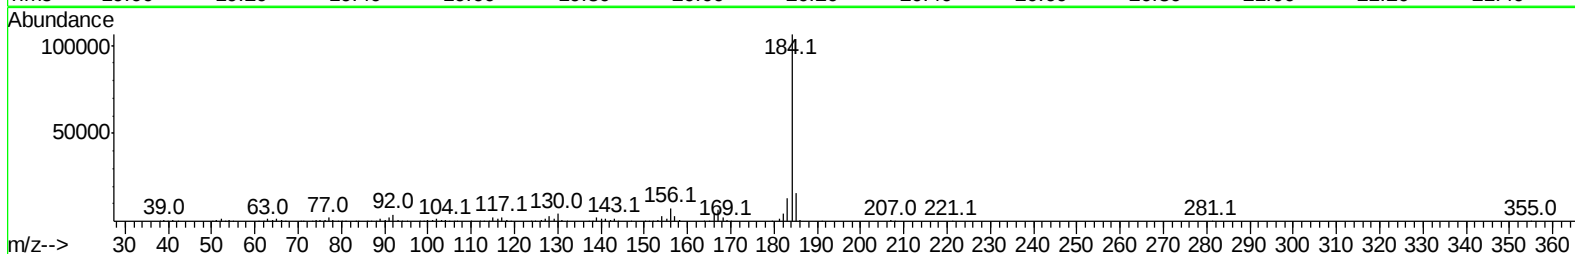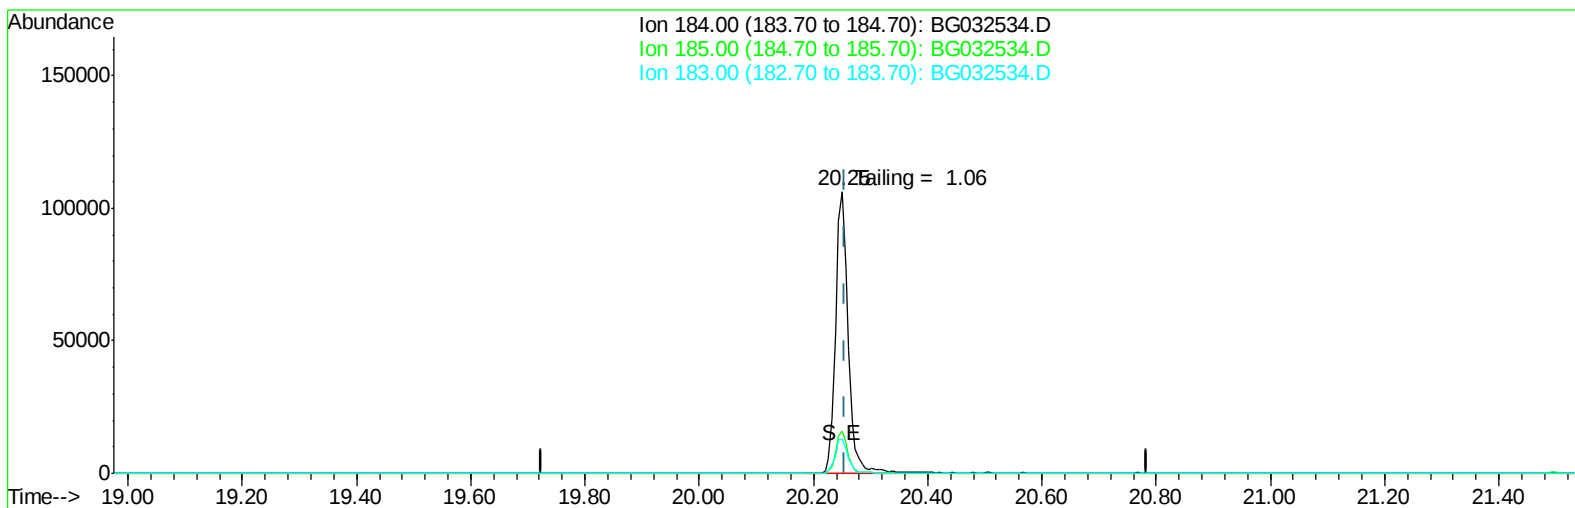

TIC: BG032534.D

(76) Benzidine

20.250min (-0.005) 56791.94ng

response 160584

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.99
183.00	13.30	12.36
0.00	0.00	0.00