
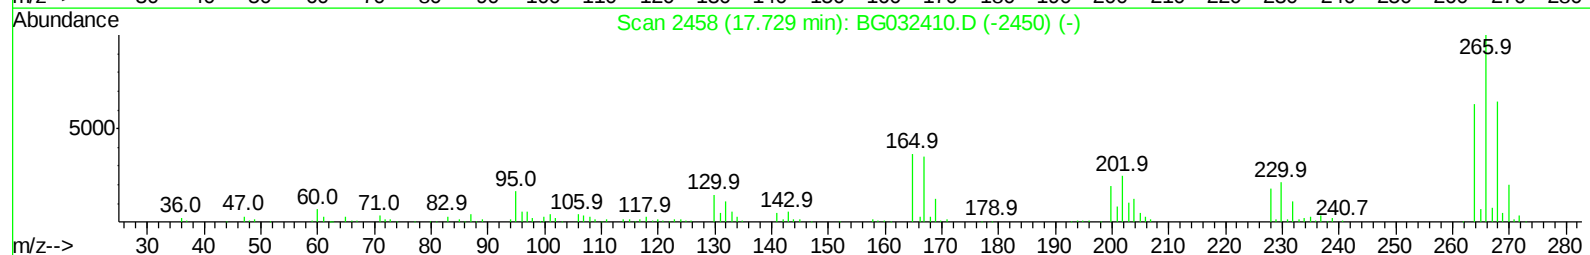
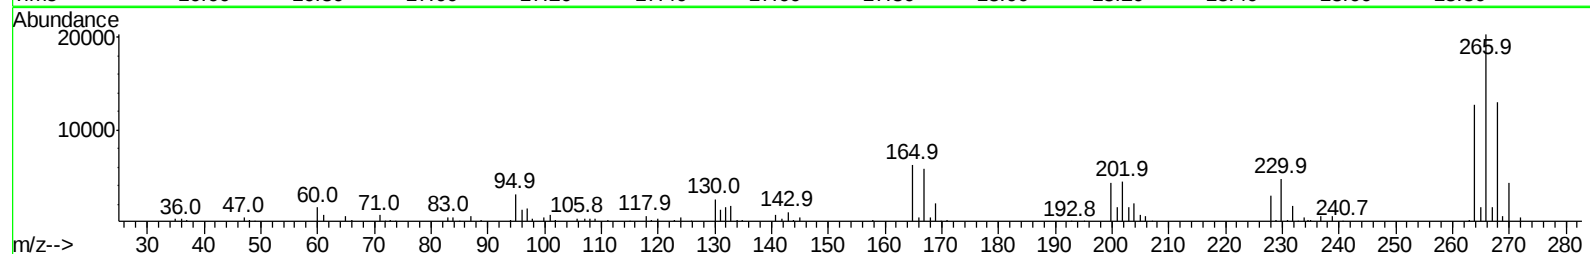


Data Path : U:\HPCHEM1\BNA G\DATA\BG020518\
Data File : BG032546.D
Acq On : 5 Feb 2018 22:48
Operator : SJ/JU
Sample : DFTPP
Misc : MDL8PPM
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 08:35:40 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 29 15:32:55 2018
Response via : Initial Calibration

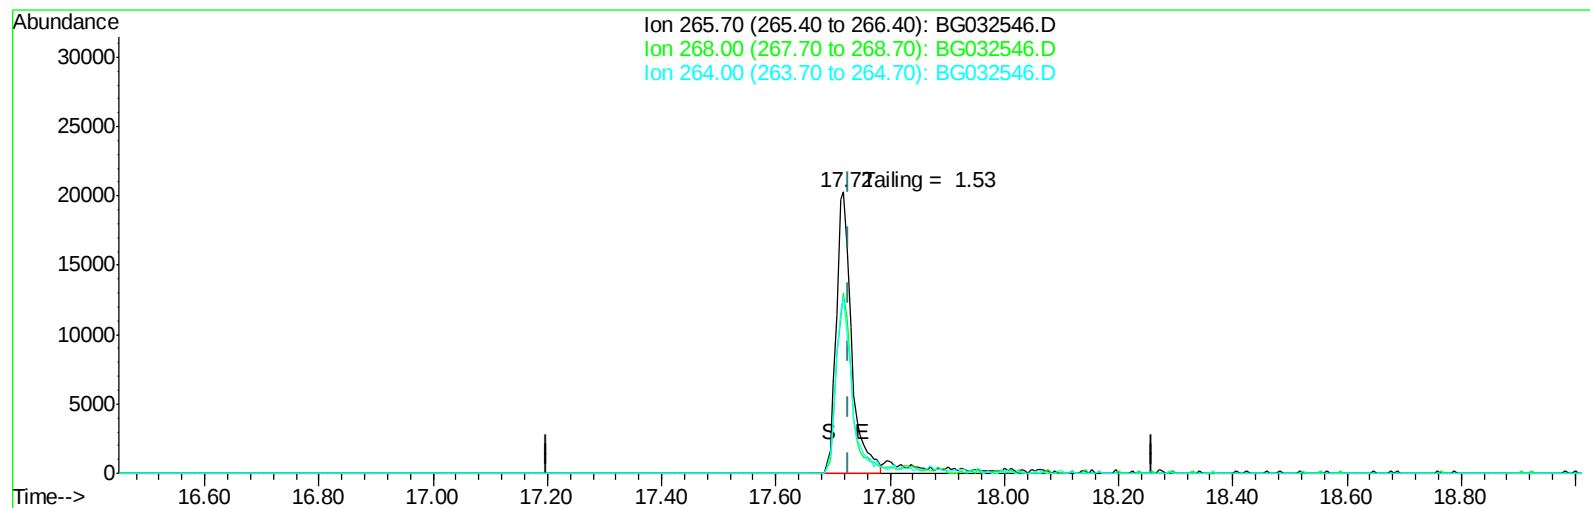

TIC: BG032546.D

(69) Pentachlorophenol (C)




17.719min (-0.010) 12902.50ng

response 37634

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.20
264.00	62.00	62.90
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA G\DATA\BG020518\
Data File : BG032546.D
Acq On : 5 Feb 2018 22:48
Operator : SJ/JU
Sample : DFTPP
Misc : MDL8PPM
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 08:35:40 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 29 15:32:55 2018
Response via : Initial Calibration

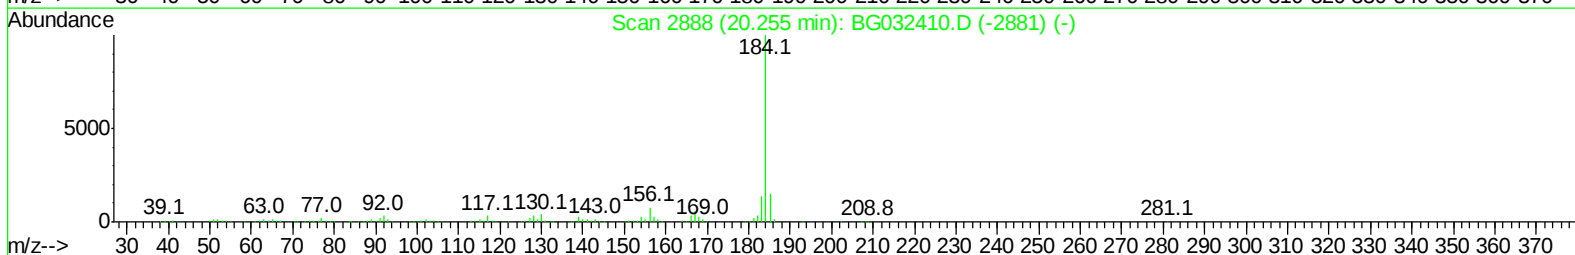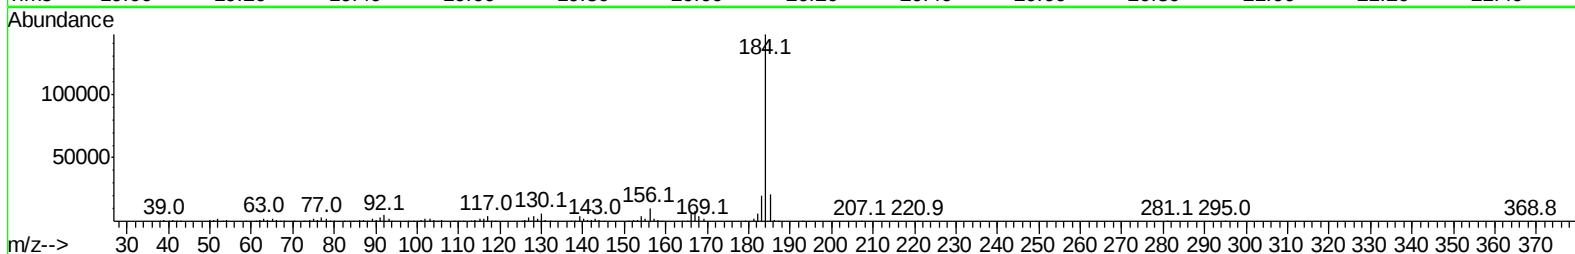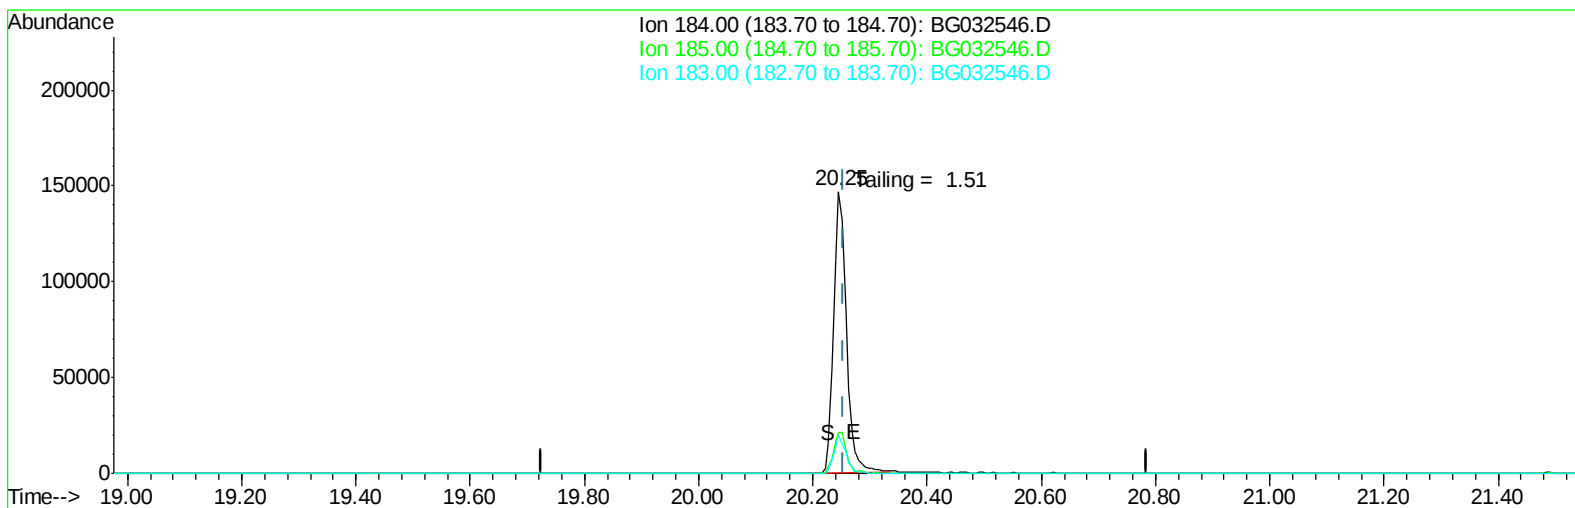

TIC: BG032546.D

(76) Benzidine

20.245min (-0.010) 210734.46ng

response 231727

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.72
183.00	13.30	13.63
0.00	0.00	0.00