

Data Path : U:\HPCHEM1\BNA G\DATA\BG020518\
Data File : BG032562.D
Acq On : 6 Feb 2018 8:47
Operator : SJ/JU
Sample : PB106300BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB106300BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG012918.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.151	479	487	504	rBV	225491	456805	20.23%	5.343%
2	7.826	764	772	795	rBV	206416	430896	19.09%	5.040%
3	8.219	832	839	855	rBV	293245	580066	25.69%	6.785%
4	8.707	914	922	932	rBV2	46252	95796	4.24%	1.120%
5	9.042	970	979	990	rBV	201858	399864	17.71%	4.677%
6	9.906	1118	1126	1138	rBV	122832	259798	11.51%	3.039%
7	11.586	1404	1412	1424	rBV	84084	170918	7.57%	1.999%
8	13.965	1810	1817	1832	rBV	698626	1168765	51.77%	13.670%
9	15.340	2044	2051	2063	rBV2	166028	287759	12.75%	3.366%
10	16.815	2296	2302	2318	rBV	465634	839114	37.17%	9.814%
11	18.072	2510	2516	2531	rBV2	251251	403408	17.87%	4.718%
12	20.611	2942	2948	2963	rBV	1700992	2257566	100.00%	26.405%
13	22.397	3244	3252	3264	rBV2	302812	582180	25.79%	6.809%
14	26.069	3863	3877	3891	rBV2	184460	616814	27.32%	7.214%


Sum of corrected areas: 8549749

Data Path : U:\HPCHEM1\BNA G\DATA\BG020518\
Data File : BG032562.D
Acq On : 6 Feb 2018 8:47
Operator : SJ/JU
Sample : PB106300BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB106300BL

Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

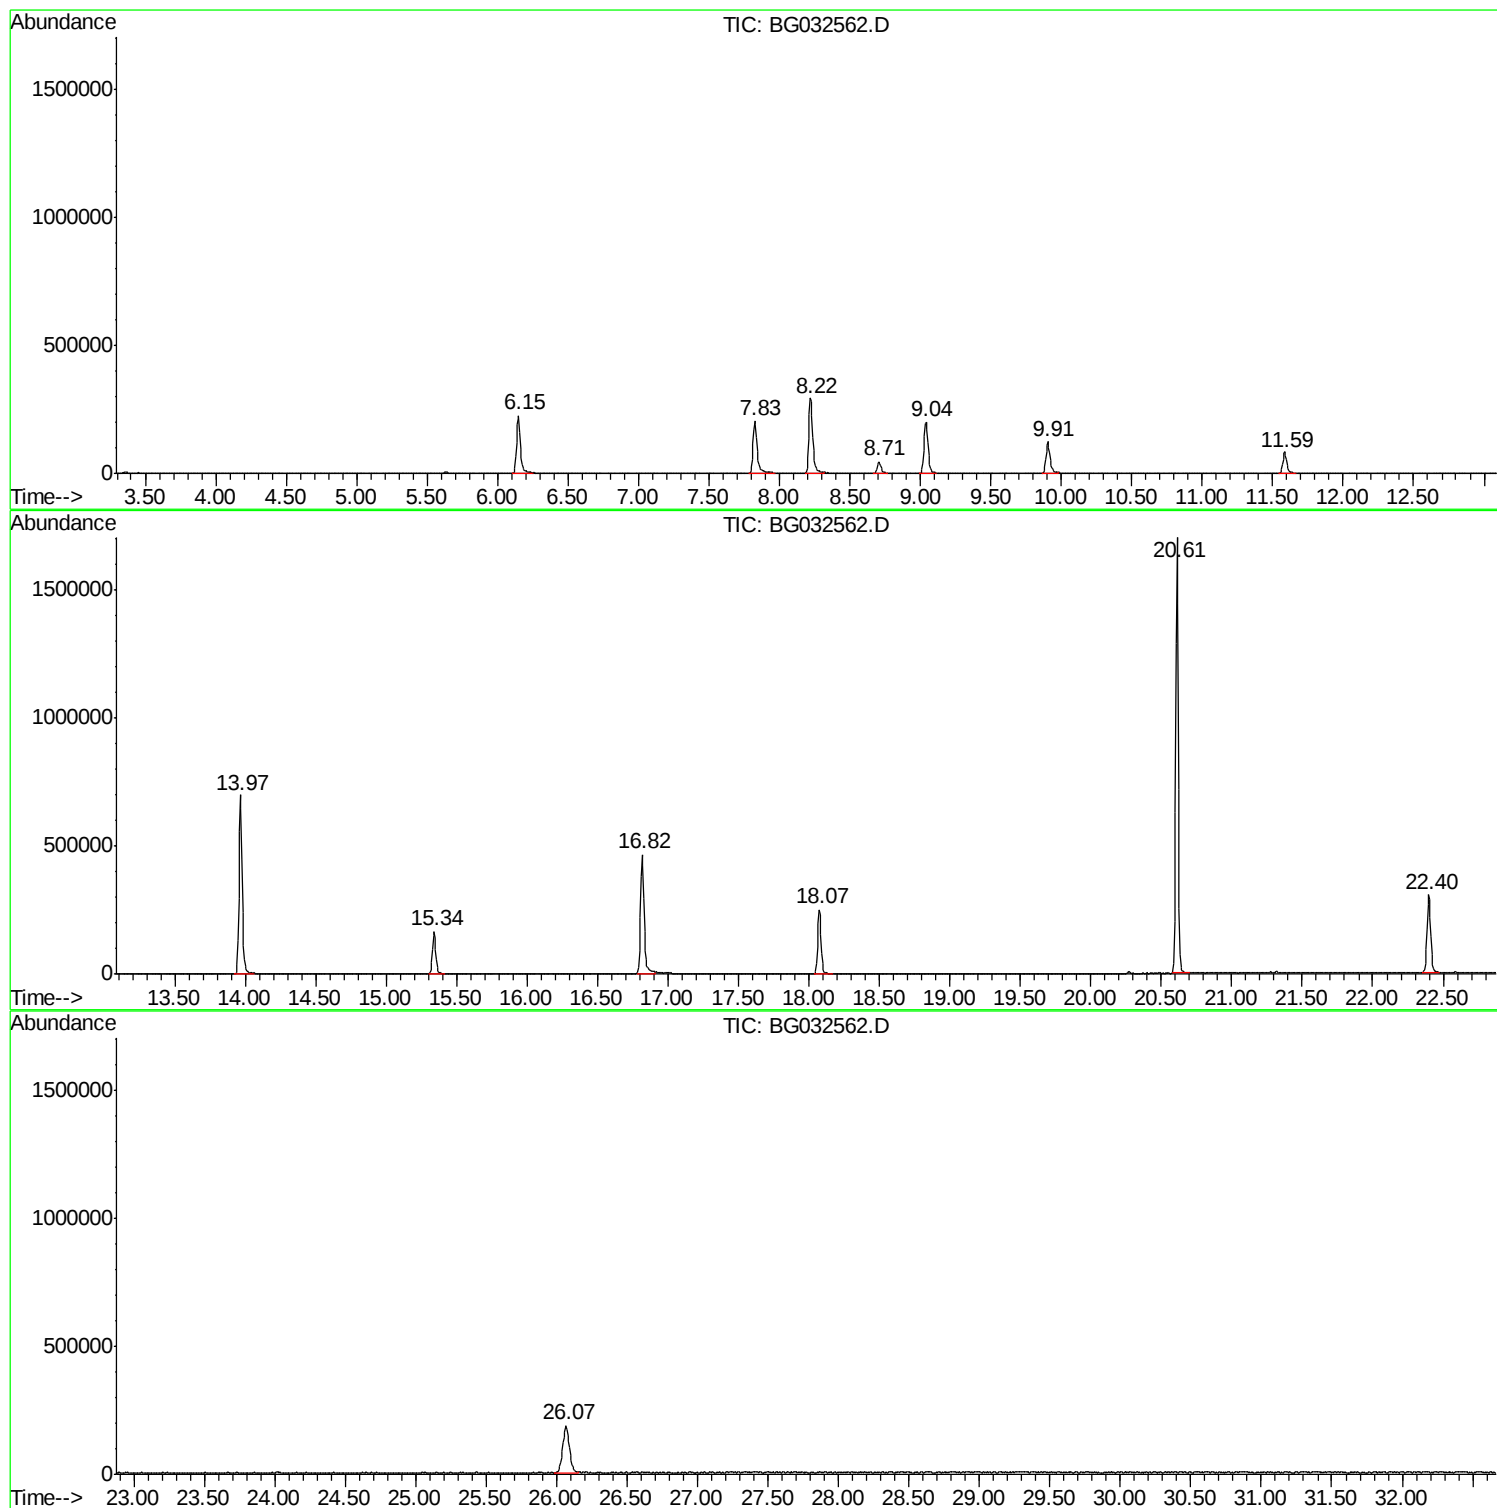

Data_Path : U:\HPCHEM1\BNA_G\DATA\BG020518\
Data_File : BG032562.D
Acq_On : 6_Feb_2018 8:477
Operator : SJ/JUU
Sample : PB106300BLL
Misc :
ALS_Vial : 26 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
PB106300BL

Quant_Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG012918.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
