


Data Path : U:\HPCHEM1\BNA G\Data\BG020518\
 Data File : BG032546.D
 Acq On : 5 Feb 2018 22:48
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG012918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 29 15:32:55 2018

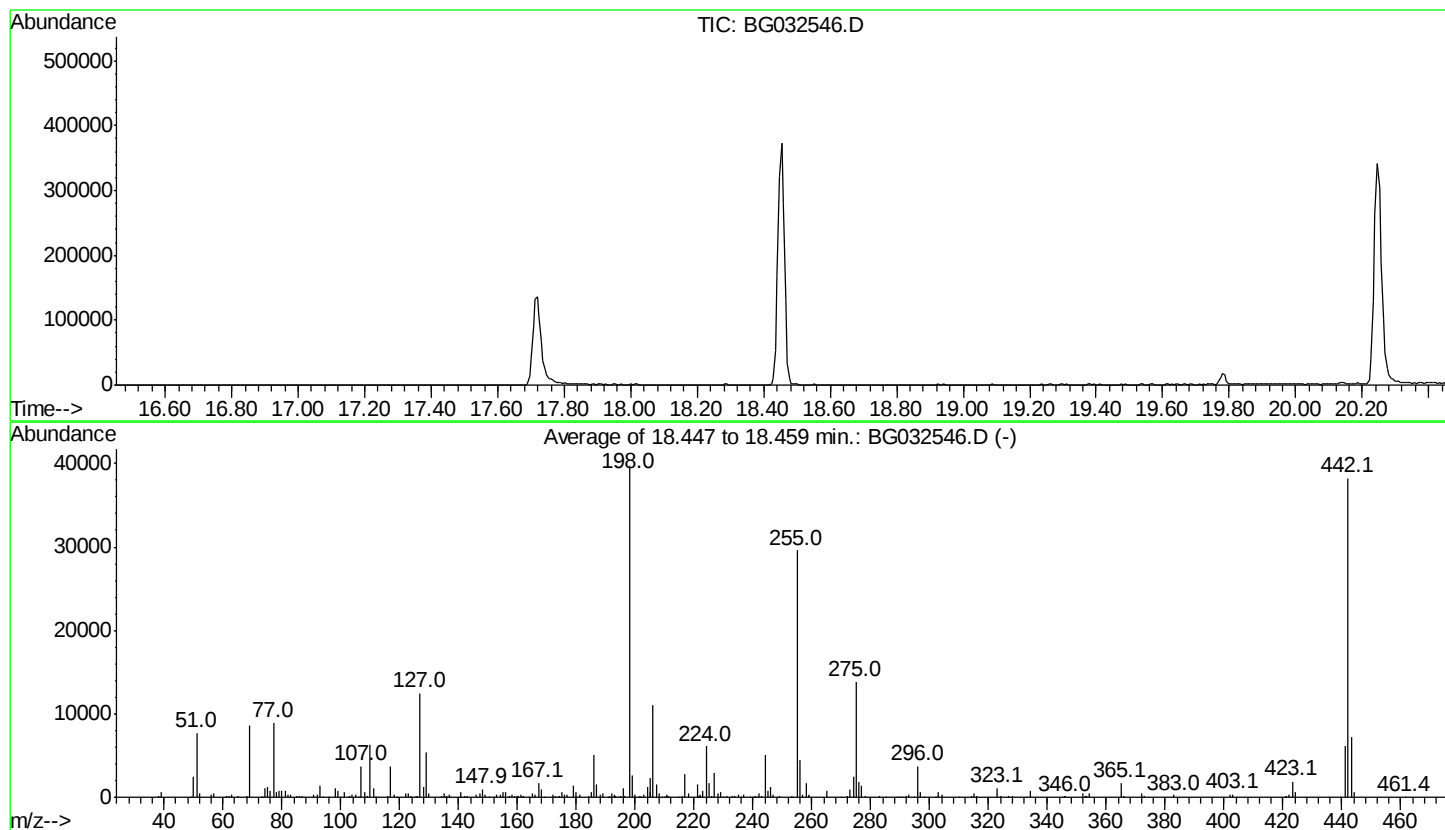

AutoFind: Scans 2580, 2581, 2582; Background Corrected with Scan 2573

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.3	7674	PASS
68	69	0.00	2	1.0	83	PASS
69	198	0.00	100	21.5	8556	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	31.3	12453	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	39749	PASS
199	198	5	9	6.5	2598	PASS
275	198	10	60	34.9	13863	PASS
365	198	1	100	4.4	1756	PASS
441	442	0.01	24	16.2	6211	PASS
442	198	50	100	96.2	38240	PASS
443	442	15	24	19.1	7288	PASS