
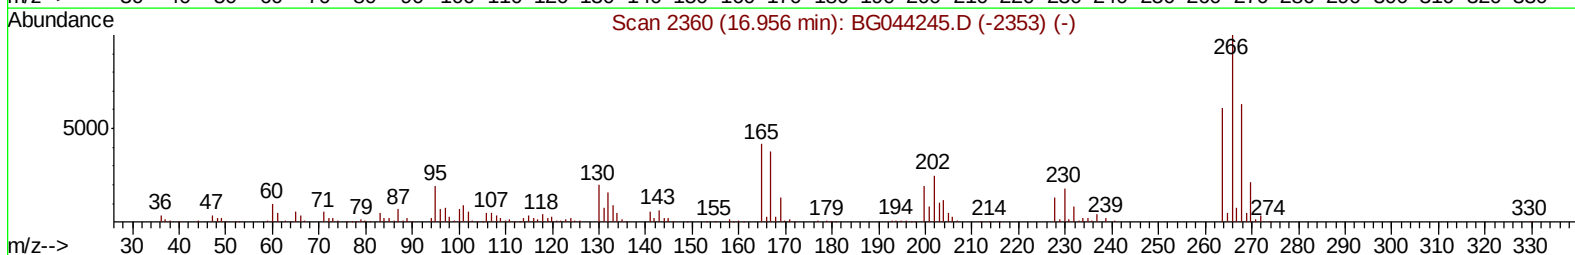
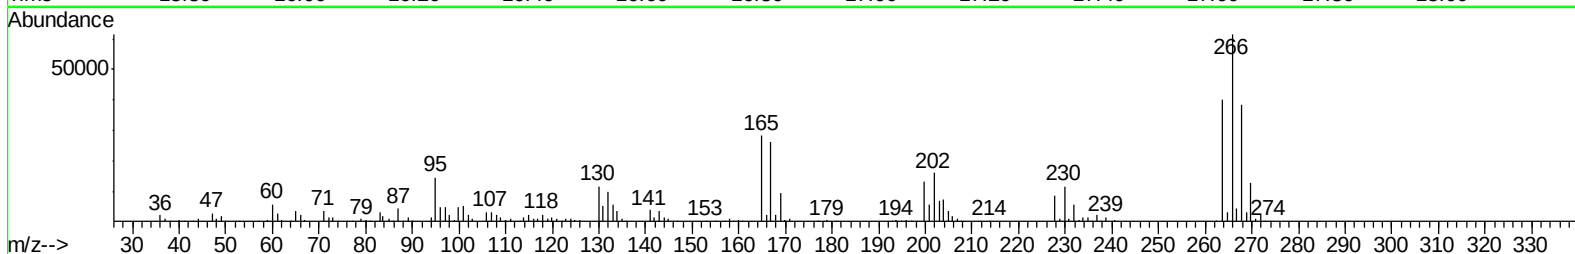


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG020520\
Data File : BG044300.D
Acq On : 5 Feb 2020 11:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 03:12:07 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG013020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 30 16:05:09 2020
Response via : Initial Calibration

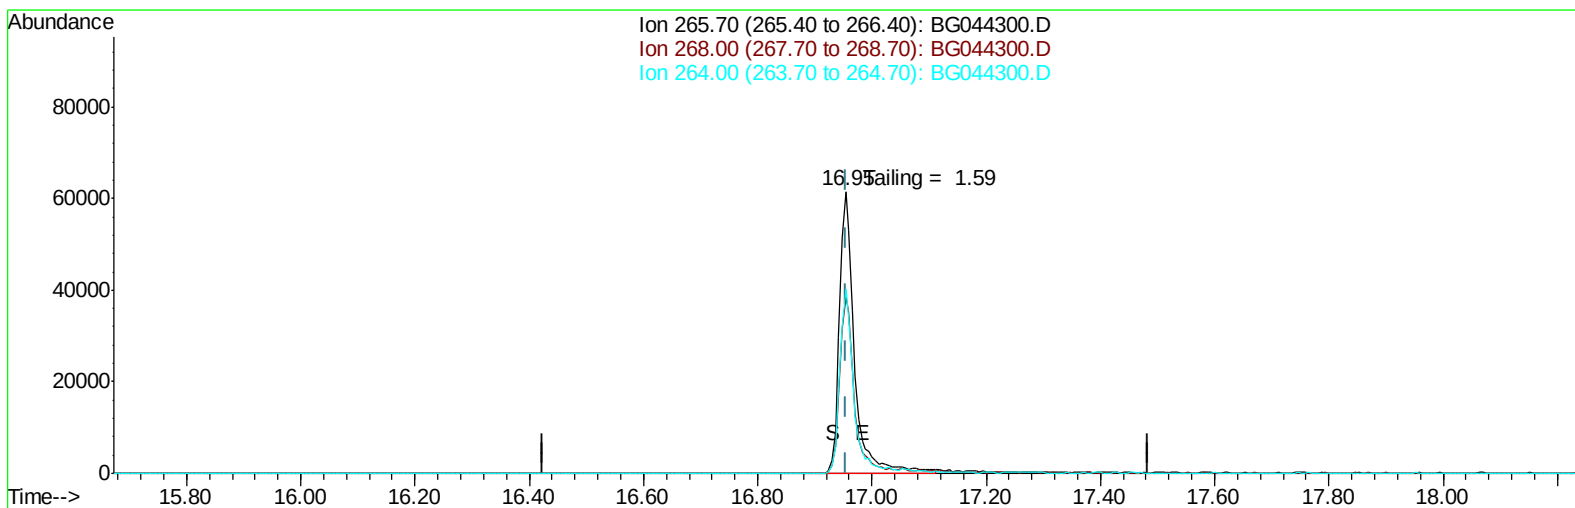

TIC: BG044300.D

(70) Pentachlorophenol (C)




16.953min (-0.002) 36614.37ng

response 111257

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	62.76
264.00	60.90	65.39
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG020520\
 Data File : BG044300.D
 Acq On : 5 Feb 2020 11:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 06 03:12:07 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG013020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 30 16:05:09 2020
 Response via : Initial Calibration

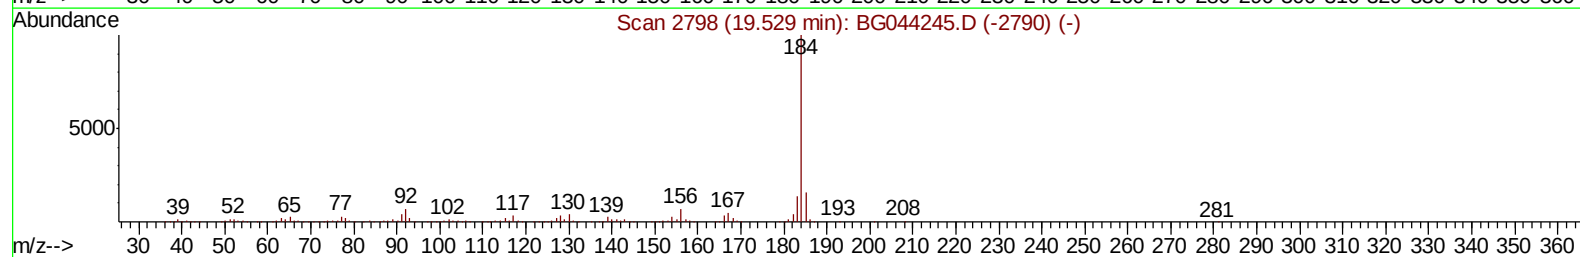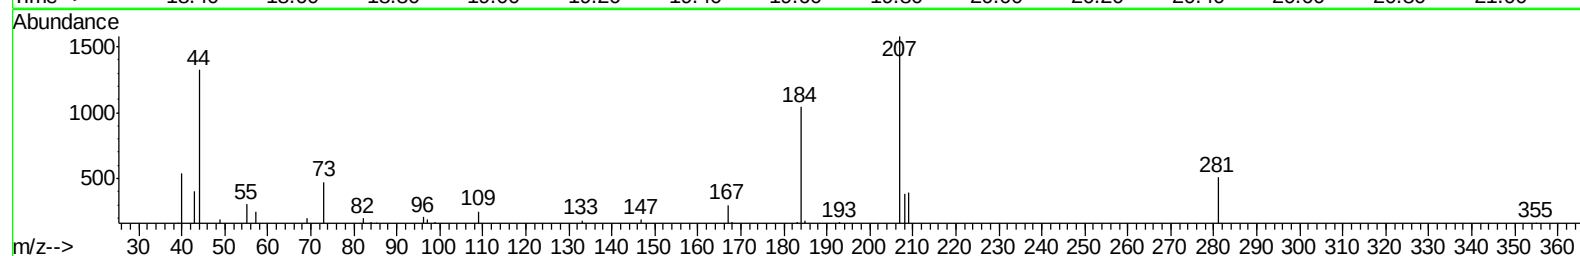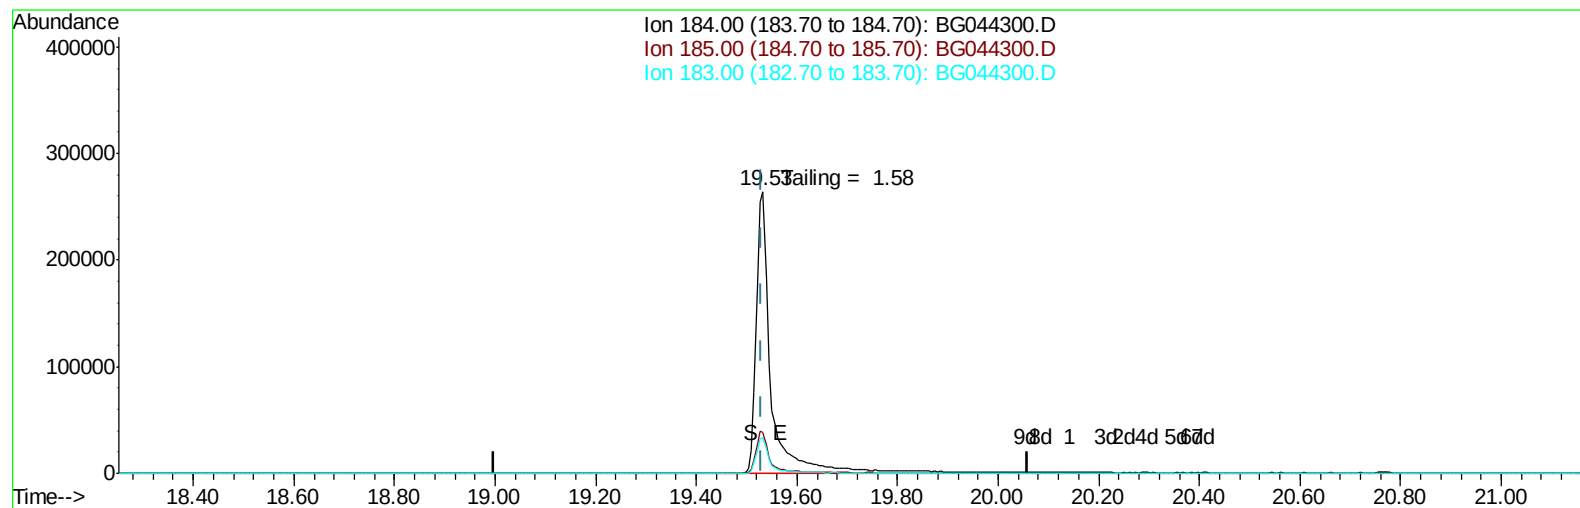

TIC: BG044300.D

(77) Benzidine

20.144min (+0.614) 221.12ng

response 460

Ion	Exp%	Act%
184.00	100	100
185.00	16.10	17.21
183.00	13.50	16.06
0.00	0.00	0.00