


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG020520\
 Data File : BG044300.D
 Acq On : 5 Feb 2020 11:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG013020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 30 16:05:09 2020

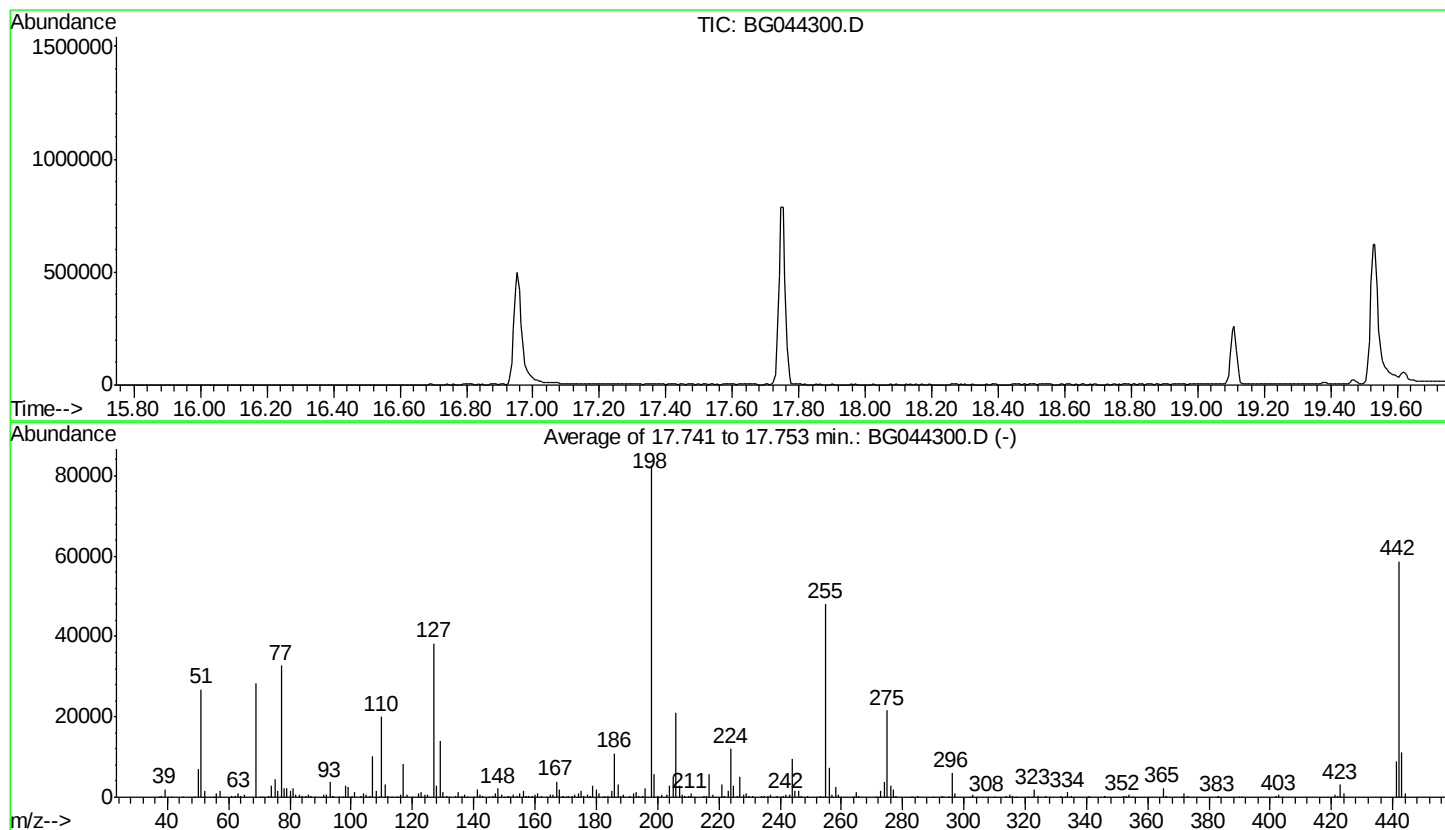

AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.5	26810	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.4	28421	PASS
70	69	0.00	2	0.5	137	PASS
127	198	10	80	46.5	38328	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	82512	PASS
199	198	5	9	6.8	5630	PASS
275	198	10	60	26.1	21538	PASS
365	198	1	100	2.8	2331	PASS
441	198	0.01	100	10.7	8826	PASS
442	198	50	100	71.2	58712	PASS
443	442	15	24	19.0	11165	PASS