
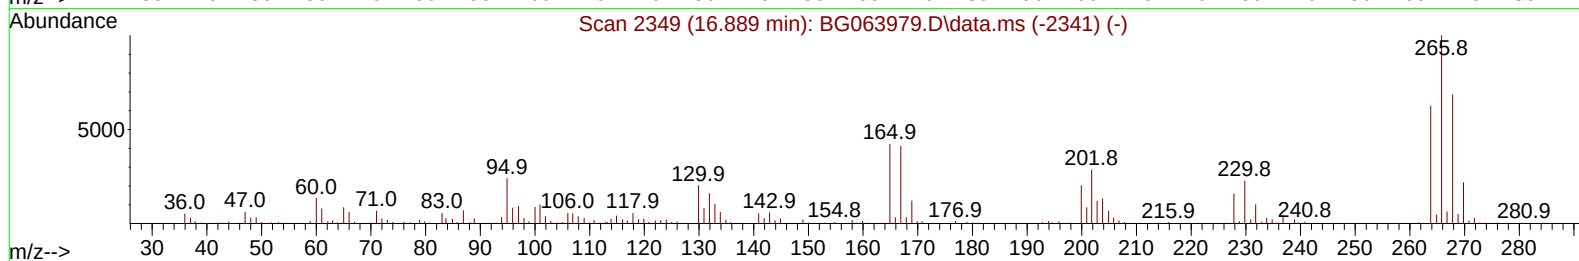
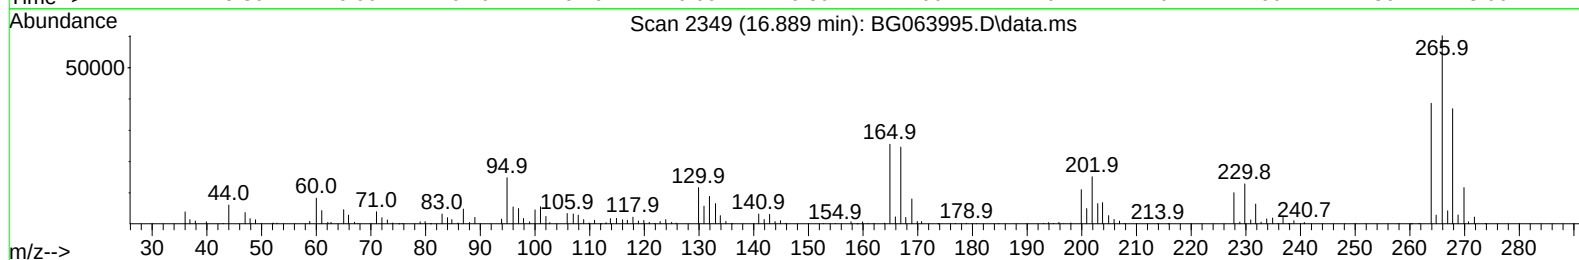


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG020525\  
Data File : BG063995.D  
Acq On : 5 Feb 2025 8:37  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 05 11:06:16 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG020325.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Feb 04 02:51:00 2025  
Response via : Initial Calibration

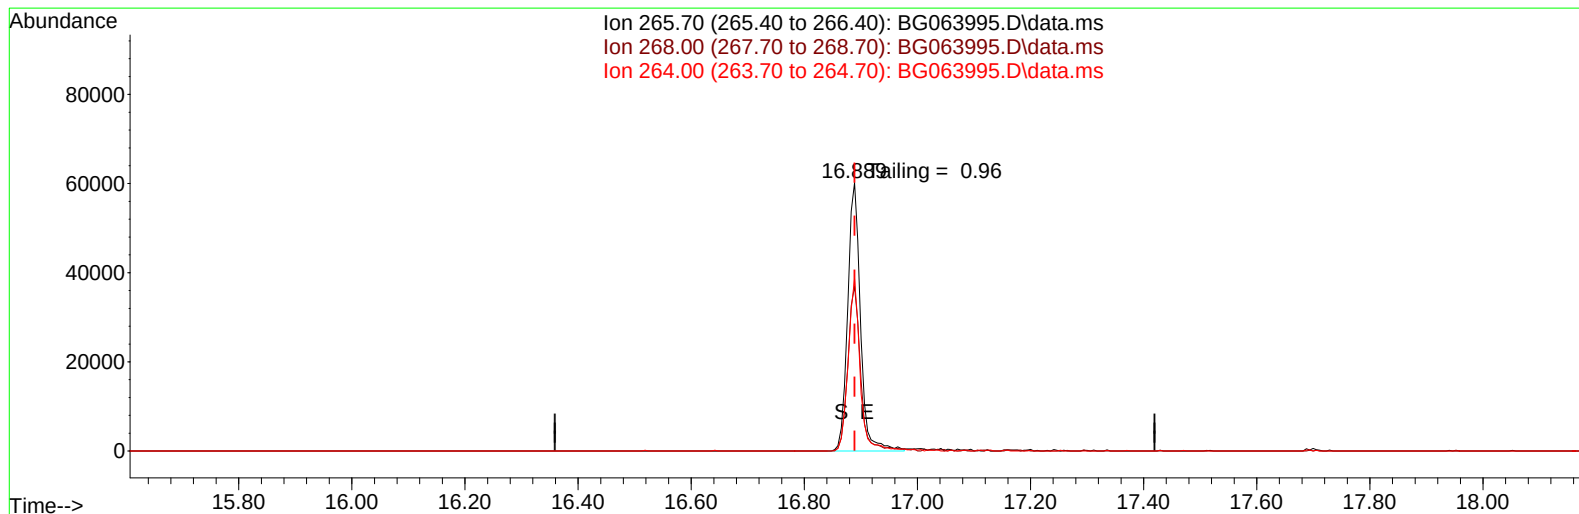

TIC: BG063995.D\data.ms

**(70) Pentachlorophenol (C)**




16.889min (-0.000) 0.00 ng

response 94760

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 68.50  | 61.29  |
| 264.00 | 62.50  | 64.15  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG020525\  
Data File : BG063995.D  
Acq On : 5 Feb 2025 8:37  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 05 11:06:16 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG020325.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Feb 04 02:51:00 2025  
Response via : Initial Calibration

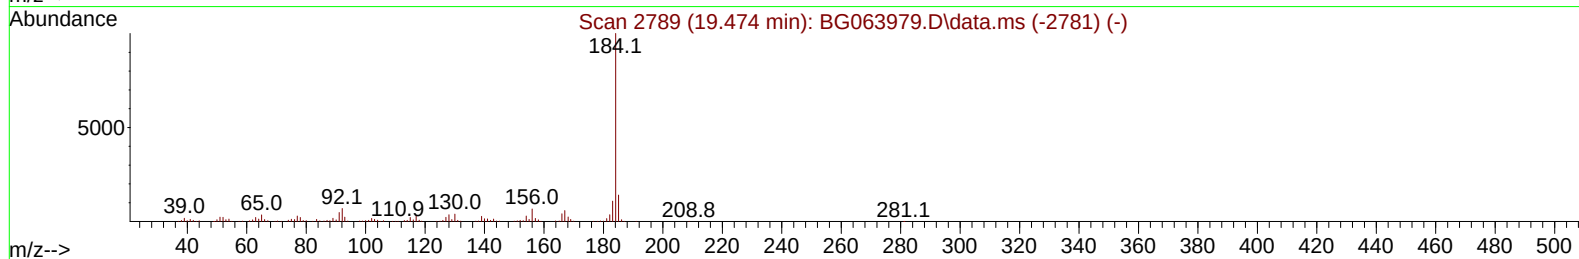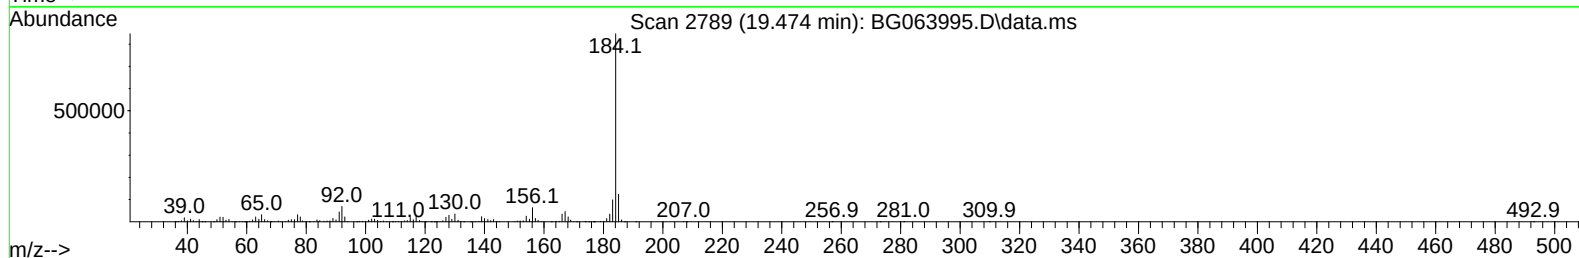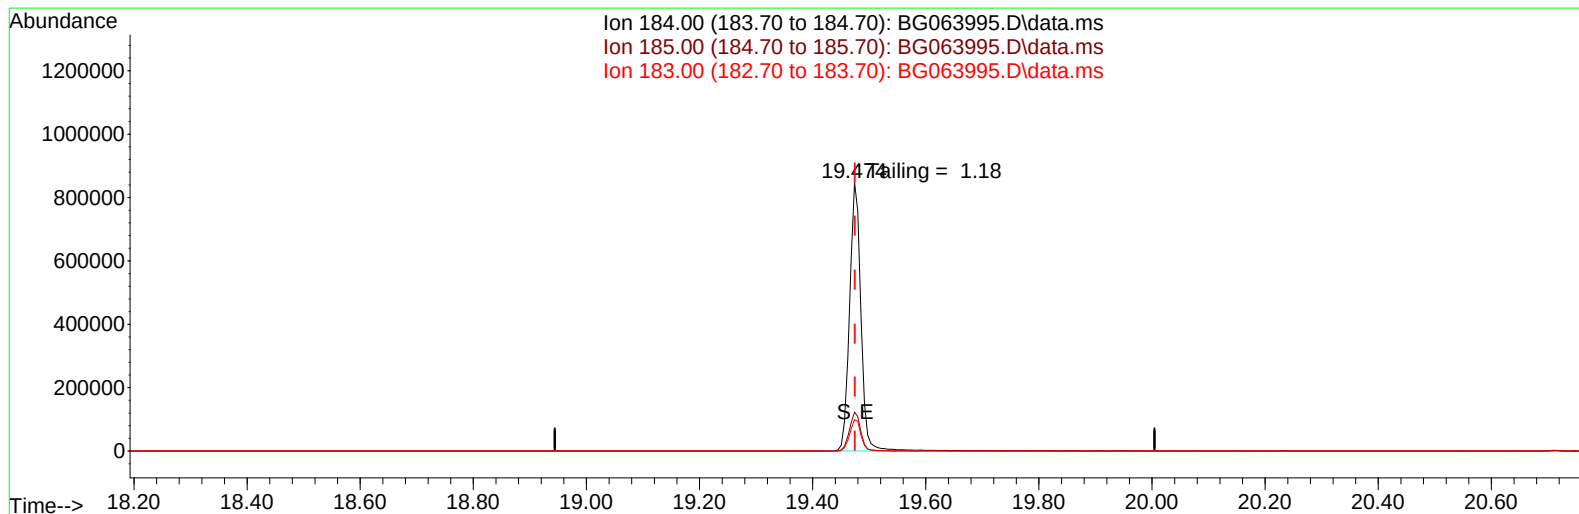

TIC: BG063995.D\data.ms

**(77) Benzidine****19.474min (-0.001) 25002.34 ng****response 1185140**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.00  | 14.54  |
| 183.00 | 10.90  | 11.68  |
| 0.00   | 0.00   | 0.00   |