
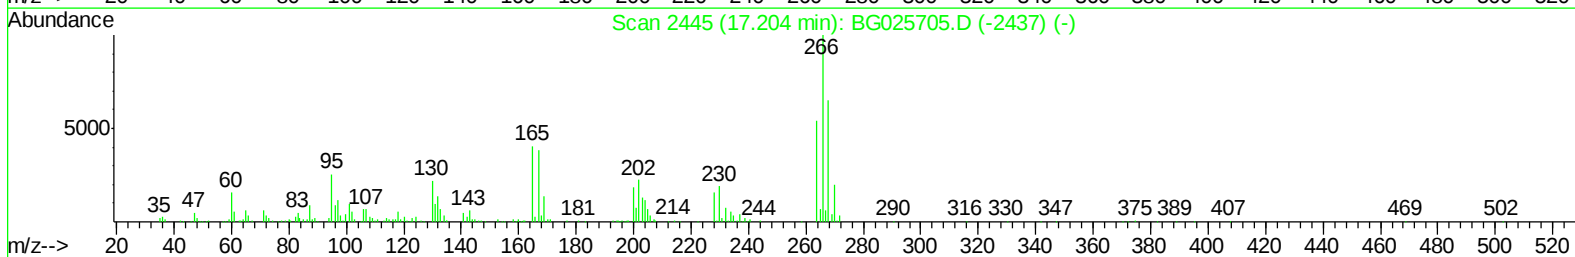
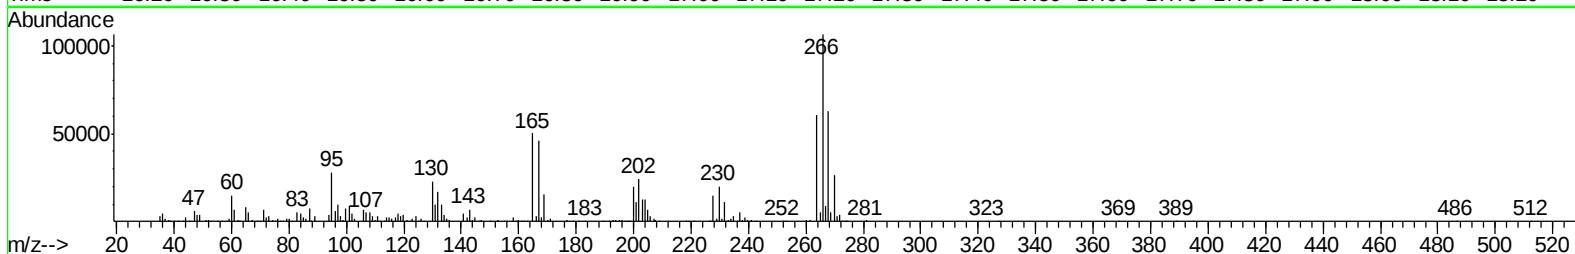


Data Path : Z:\HPCHEM1\BNA_G\Data\BG020617\
Data File : BG025805.D
Acq On : 6 Feb 2017 16:37
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 07 04:08:29 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 30 18:29:38 2017
Response via : Initial Calibration

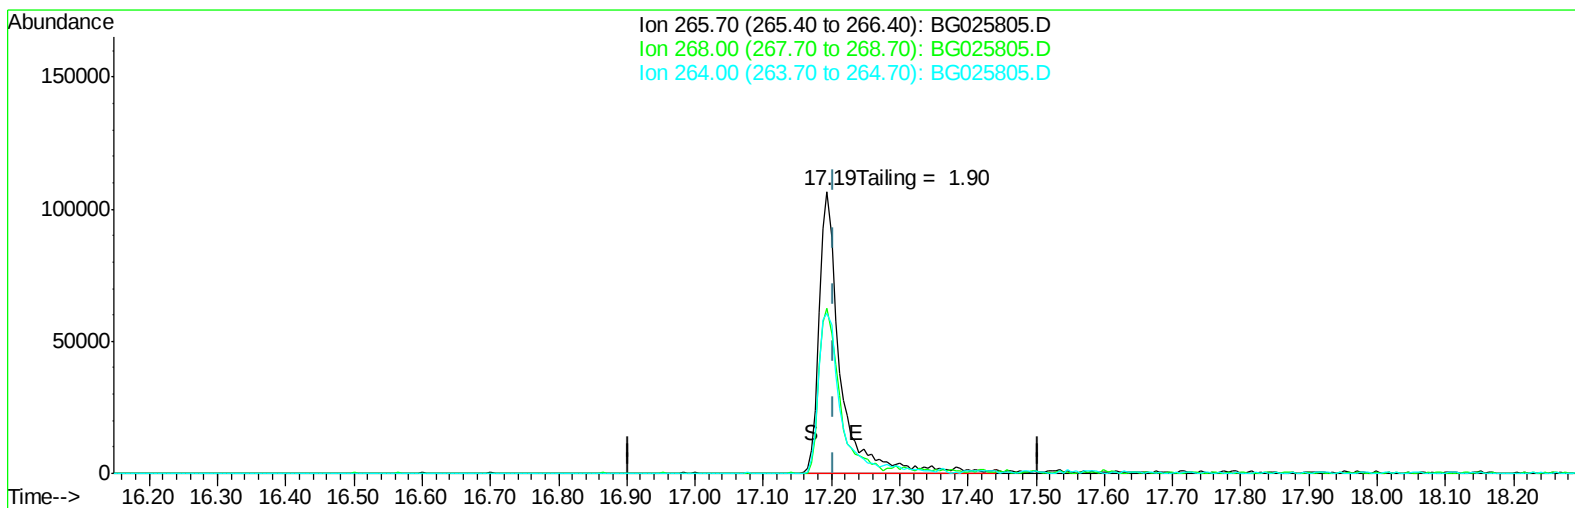

TIC: BG025805.D

(69) Pentachlorophenol (C)




17.194min (-0.010) 312145.98ng

response 215725

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	58.80
264.00	62.60	56.86
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG020617\
 Data File : BG025805.D
 Acq On : 6 Feb 2017 16:37
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 07 04:08:29 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG013017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 30 18:29:38 2017
 Response via : Initial Calibration

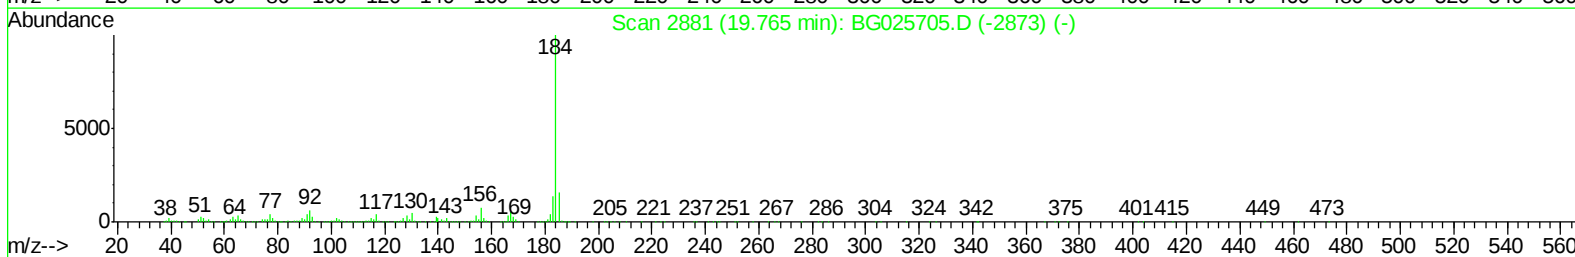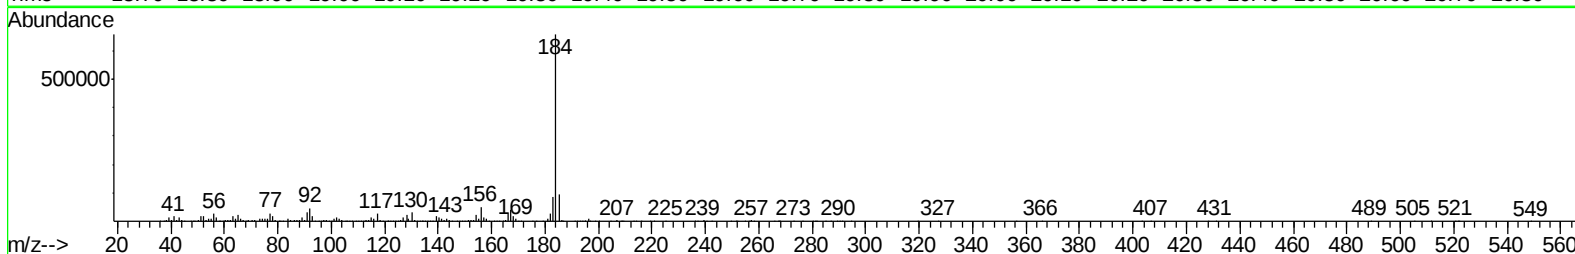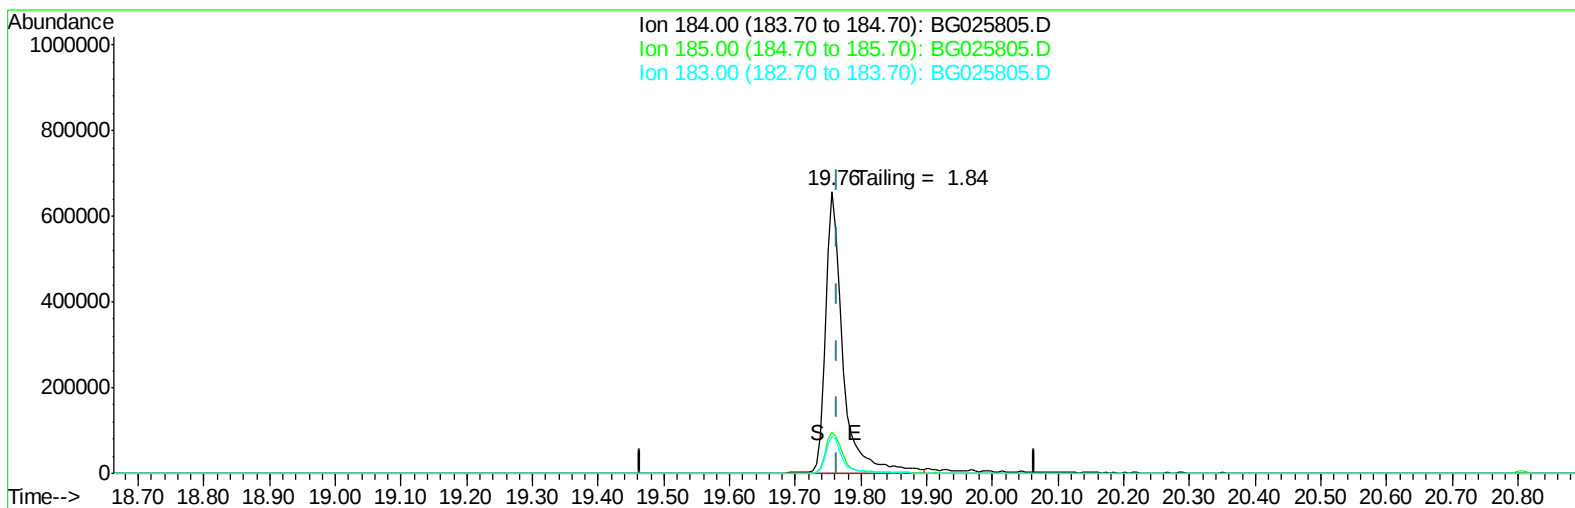

TIC: BG025805.D

(76) Benzidine

19.756min (-0.010) 569816.56ng

response 1213135

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.37
183.00	13.80	13.27
0.00	0.00	0.00