


Data Path : Z:\HPCHEM1\BNA G\DATA\BG020617\
 Data File : BG025805.D
 Acq On : 6 Feb 2017 16:37
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG013017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 30 18:29:38 2017

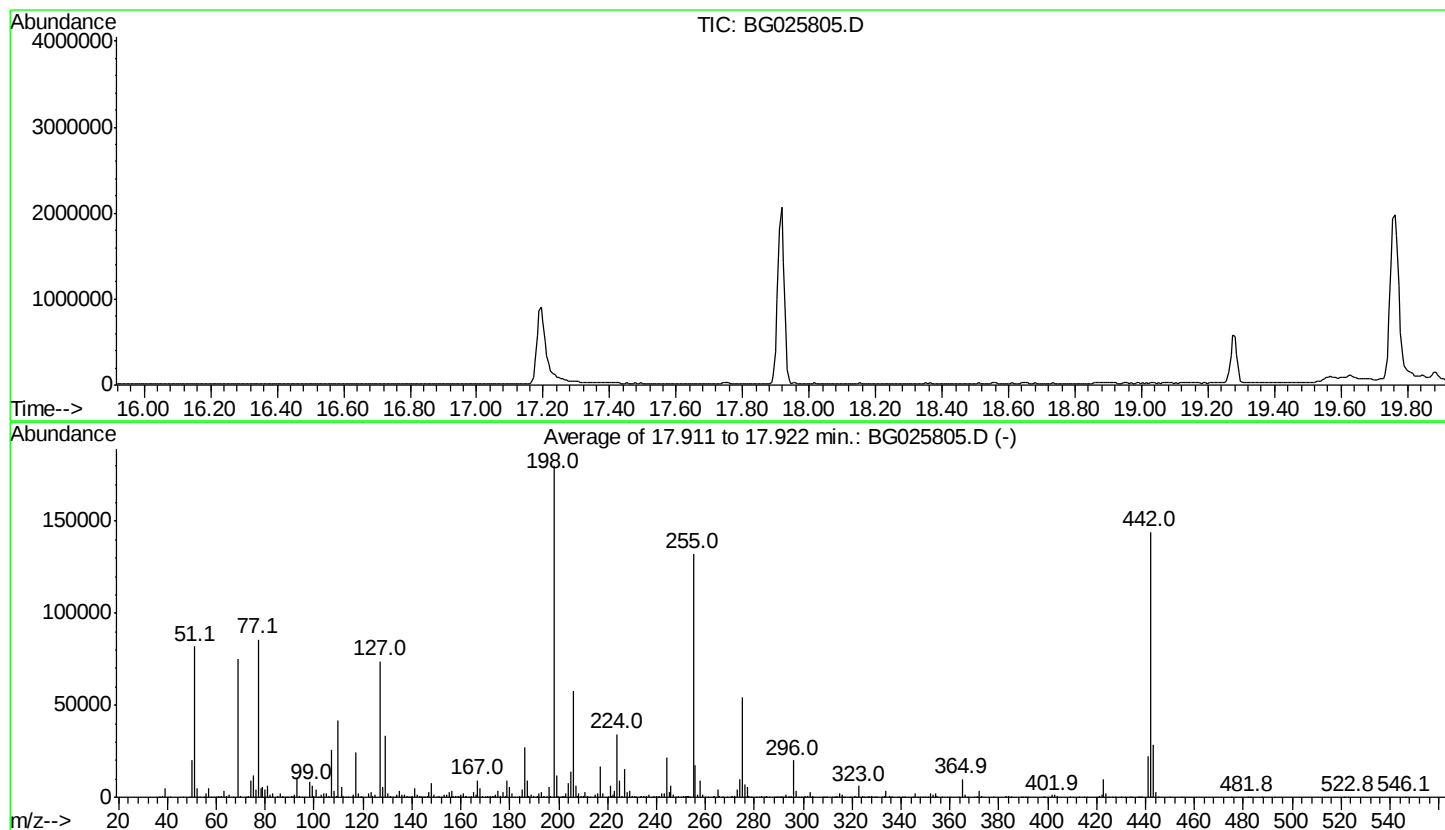

AutoFind: Scans 2565, 2566, 2567; Background Corrected with Scan 2558

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.5	81946	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	41.6	74976	PASS
70	69	0.00	2	0.6	480	PASS
127	198	10	80	41.0	73968	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	180266	PASS
199	198	5	9	6.7	12014	PASS
275	198	10	60	30.3	54594	PASS
365	198	1	100	5.5	9831	PASS
441	442	0.01	24	15.3	22109	PASS
442	198	50	100	80.0	144266	PASS
443	442	15	24	19.7	28450	PASS