
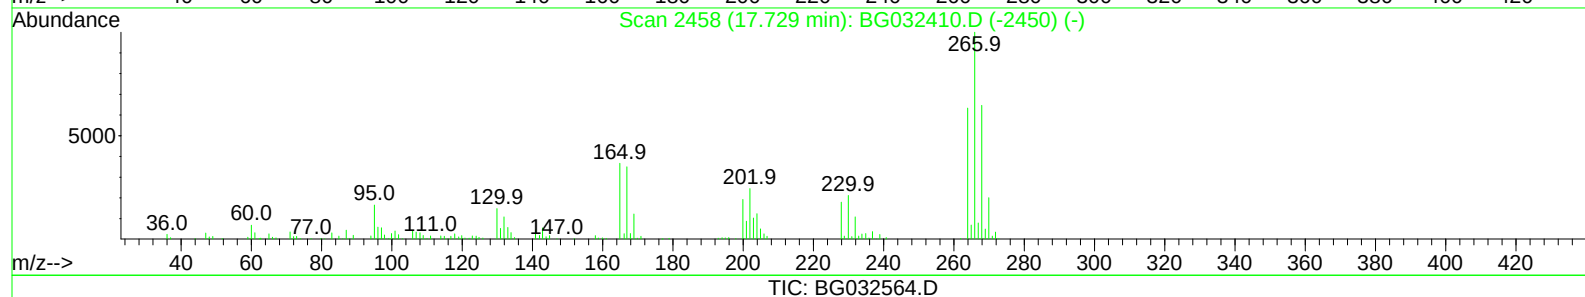
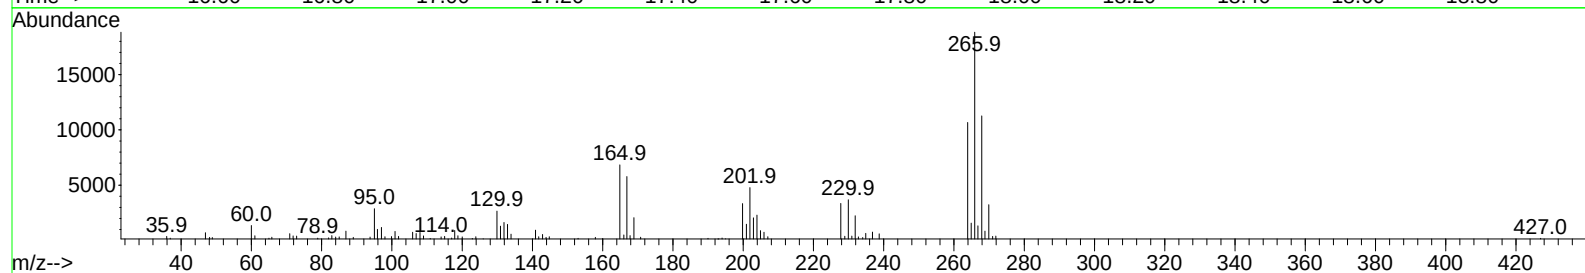


Data Path : U:\HPCHEM1\BNA G\DATA\BG020618\  
Data File : BG032564.D  
Acq On : 6 Feb 2018 13:10  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 07 06:09:03 2018  
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Feb 06 18:57:08 2018  
Response via : Initial Calibration

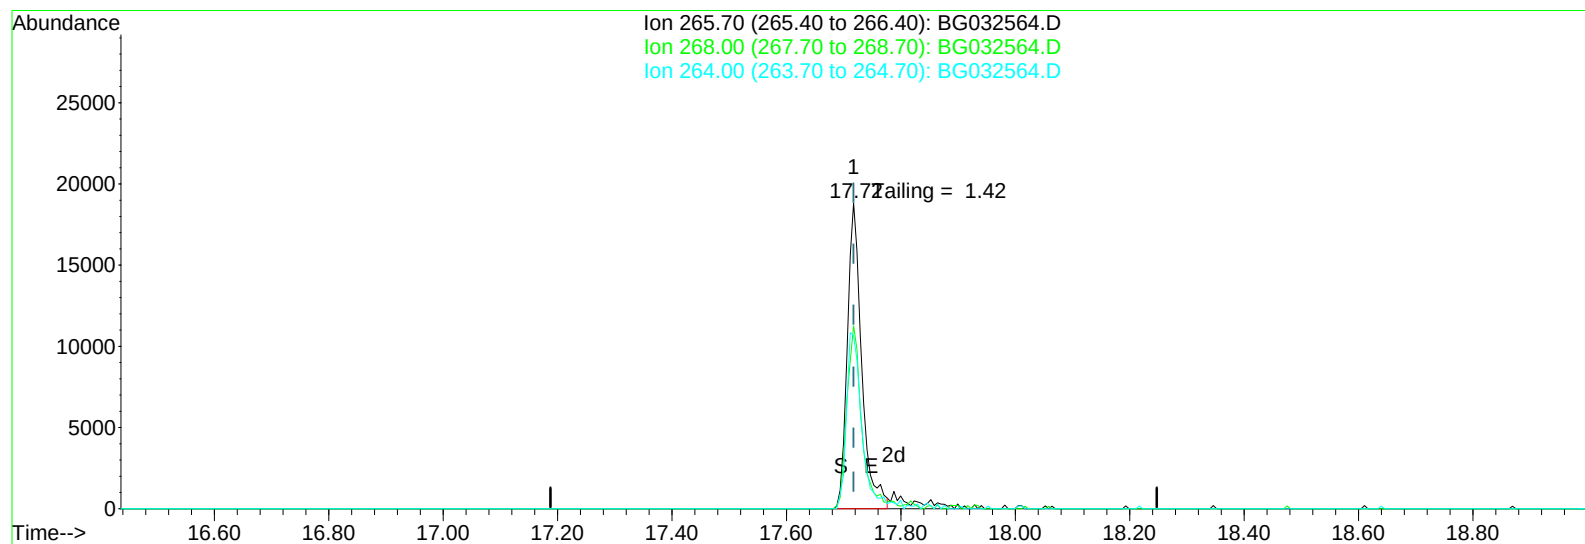

(69) Pentachlorophenol (C)




17.717min (+0.000) 46030.94ng

response 33093

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 59.80 |
| 264.00 | 62.00 | 56.65 |
| 0.00   | 0.00  | 0.00  |

Data Path : U:\HPCHEM1\BNA G\DATA\BG020618\  
 Data File : BG032564.D  
 Acq On : 6 Feb 2018 13:10  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 07 06:09:03 2018  
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Feb 06 18:57:08 2018  
 Response via : Initial Calibration

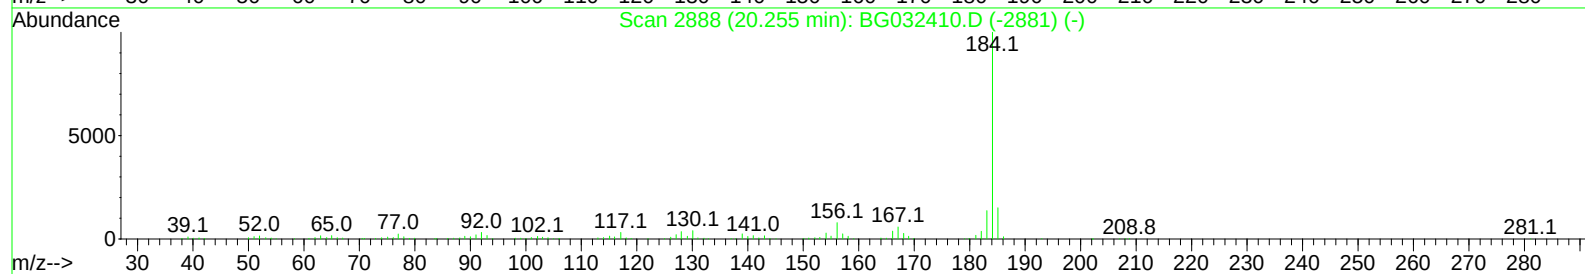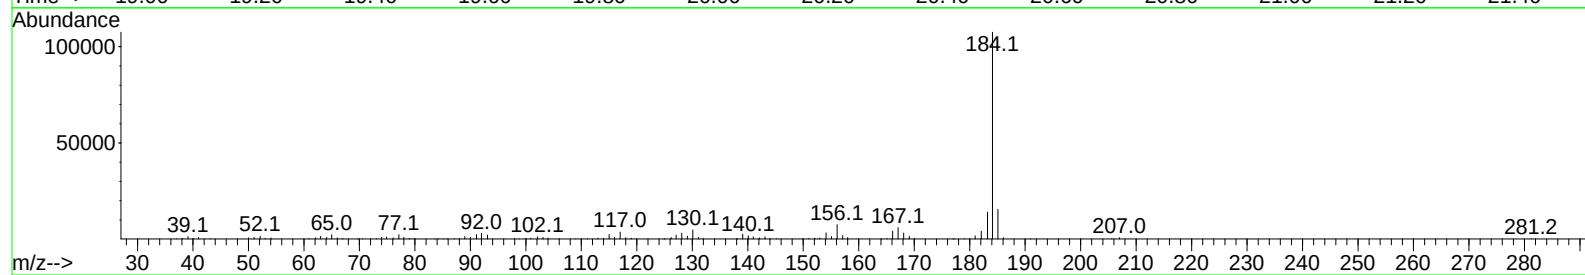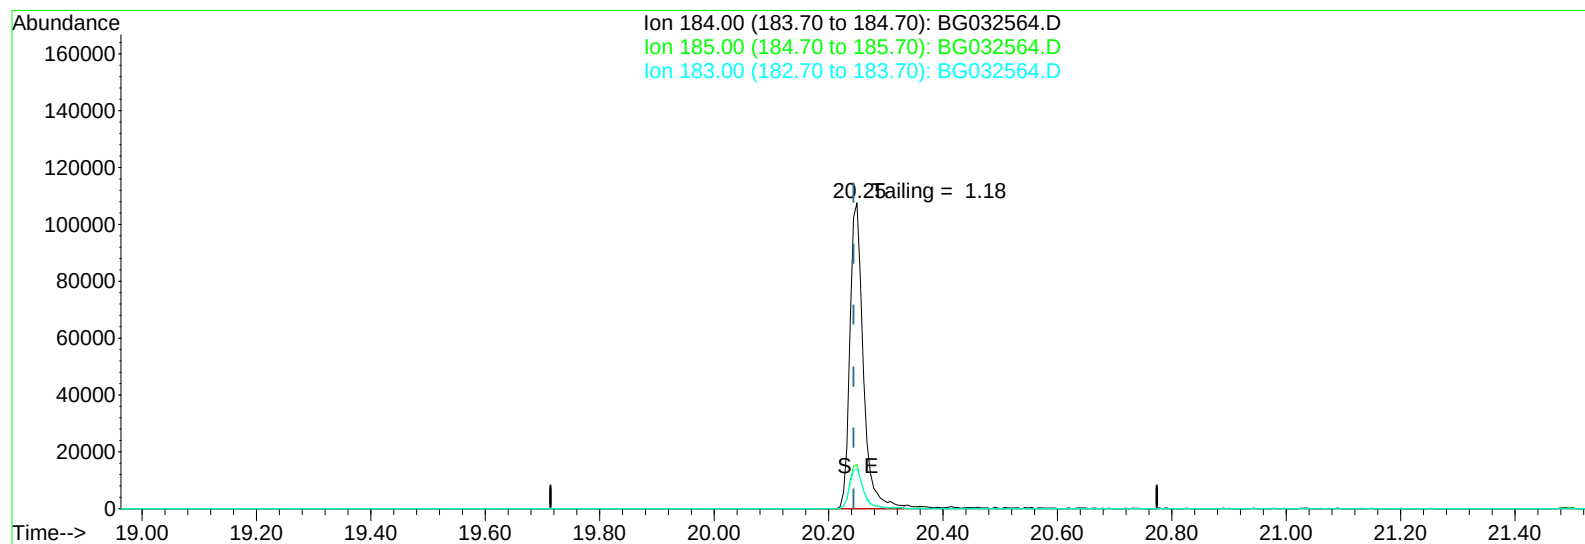

TIC: BG032564.D

(76) Benzidine

20.250min (+0.006) 0.00ng

response 175841

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 13.90 | 14.43 |
| 183.00 | 13.30 | 13.07 |
| 0.00   | 0.00  | 0.00  |