
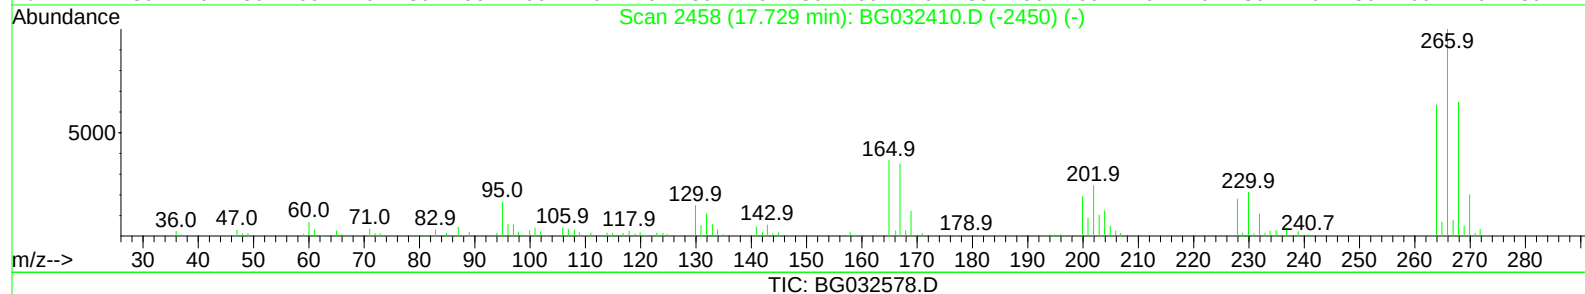
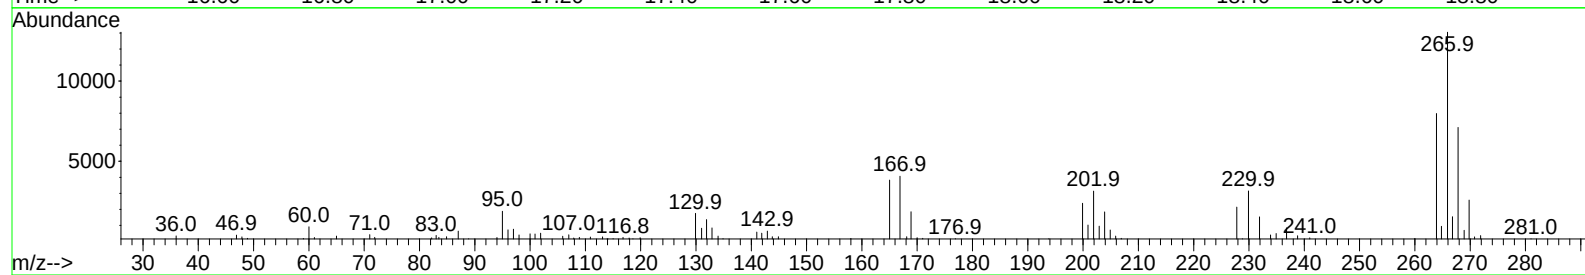


Data Path : U:\HPCHEM1\BNA G\DATA\BG020618\
Data File : BG032578.D
Acq On : 6 Feb 2018 23:26
Operator : SJ/JU
Sample : DFTPP
Misc : MDL-W-8 ppm
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 07 06:17:51 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 18:57:08 2018
Response via : Initial Calibration

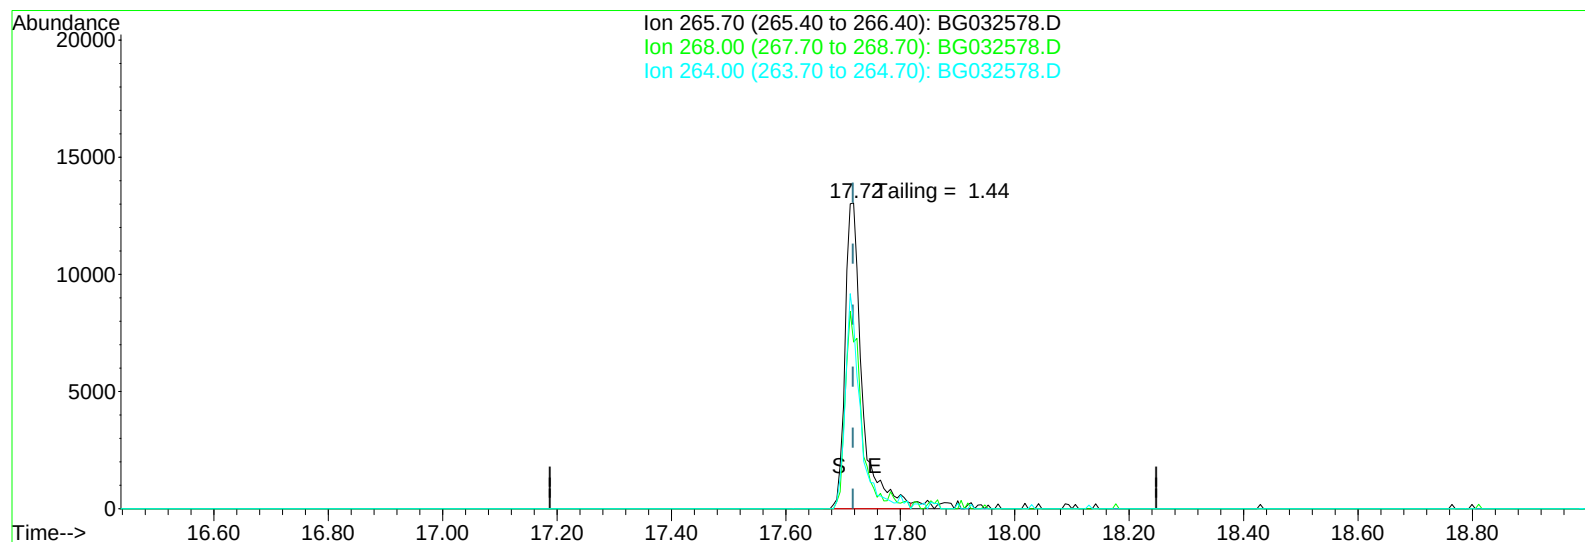

(69) Pentachlorophenol (C)




17.718min (+0.001) 0.00ng

response 26959

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	54.50
264.00	62.00	61.13
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA G\DATA\BG020618\
Data File : BG032578.D
Acq On : 6 Feb 2018 23:26
Operator : SJ/JU
Sample : DFTPP
Misc : MDL-W-8 ppm
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 07 06:17:51 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 18:57:08 2018
Response via : Initial Calibration

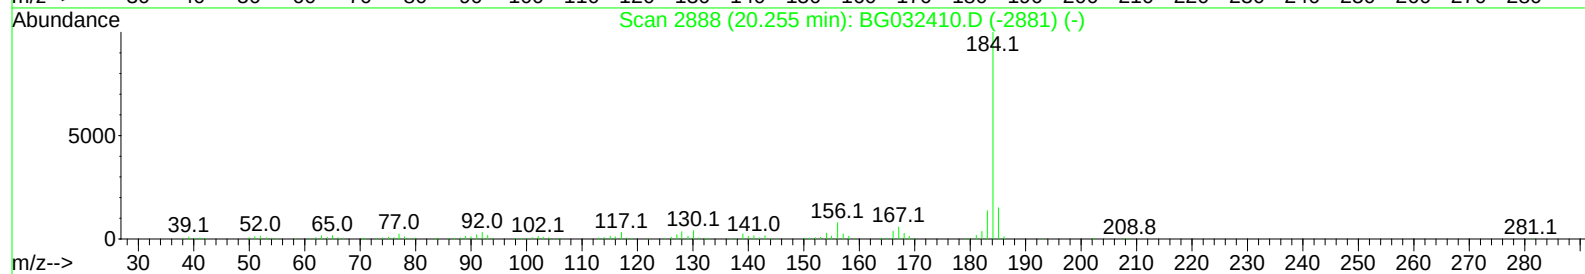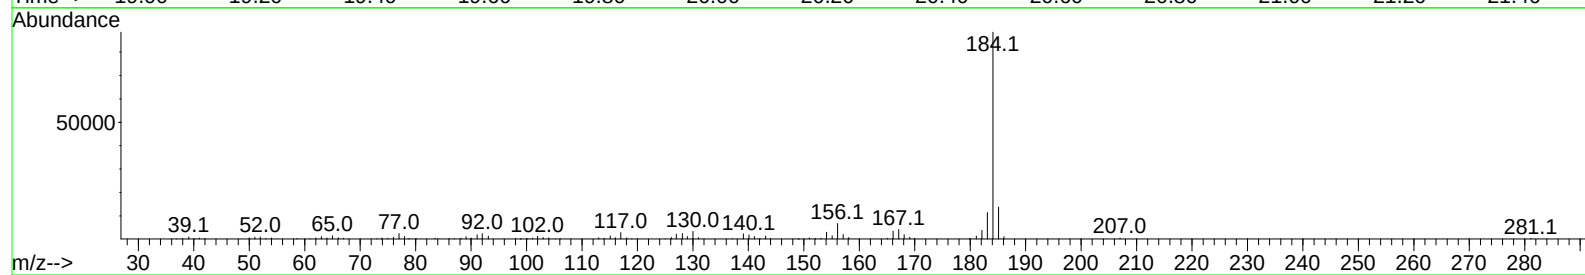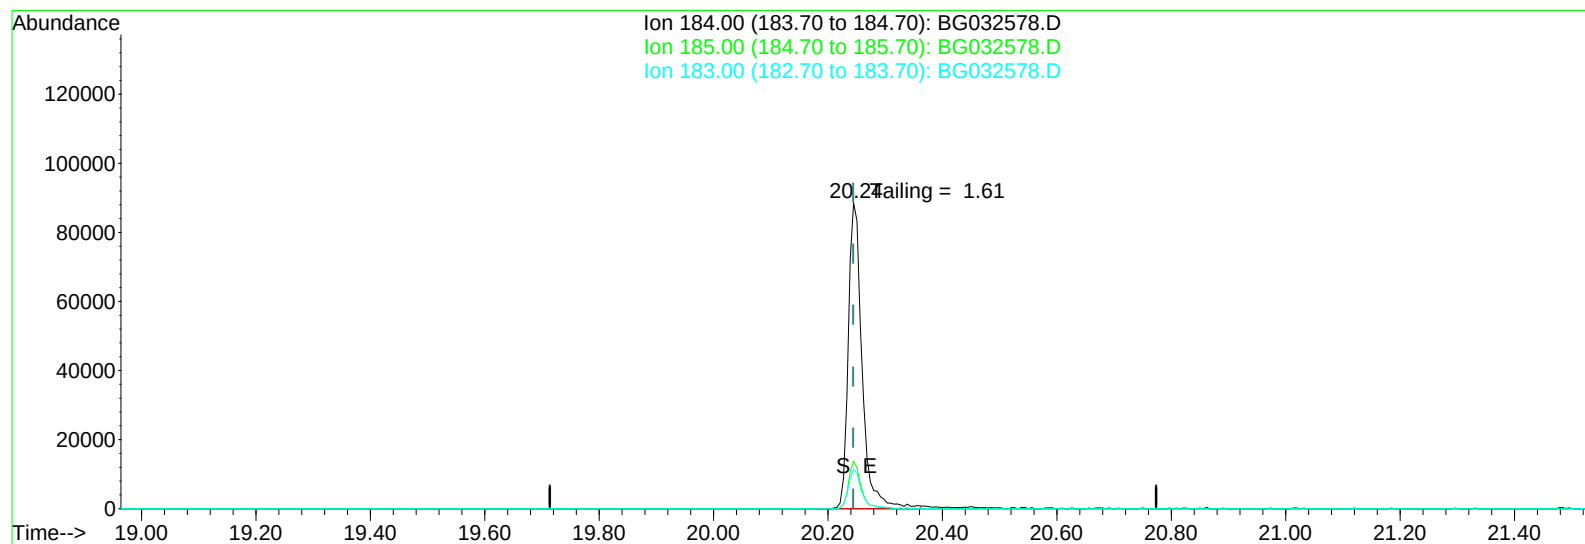

TIC: BG032578.D

(76) Benzidine

20.245min (+0.001) 110282.13ng

response 147254

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.49
183.00	13.30	12.90
0.00	0.00	0.00