


Data Path : Z:\HPCHEM1\BNA G\Data\BG020618\
 Data File : BG032564.D
 Acq On : 6 Feb 2018 13:10
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG012918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 06 18:57:08 2018

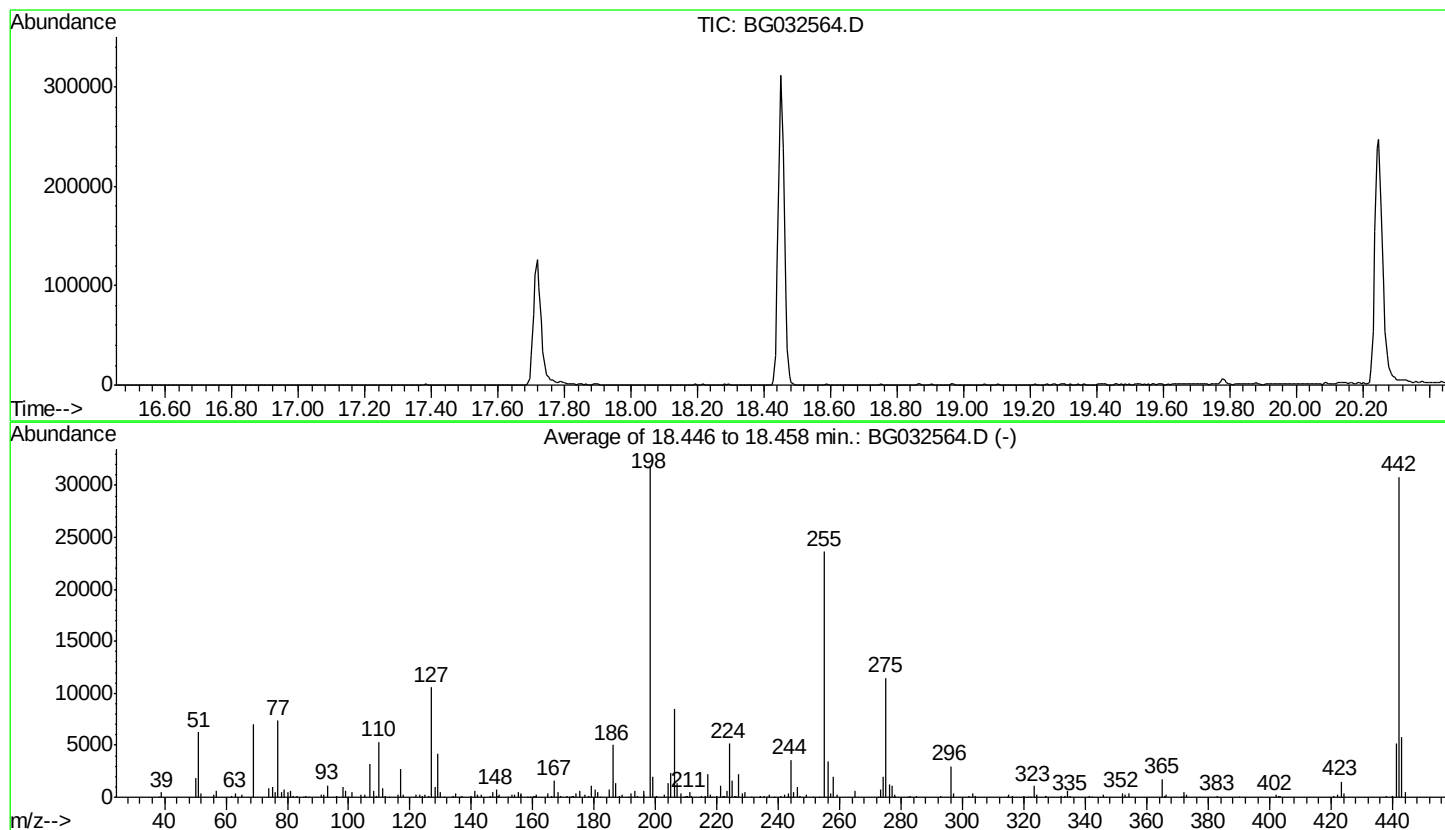

AutoFind: Scans 2580, 2581, 2582; Background Corrected with Scan 2573

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.6	6256	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	22.1	7040	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	33.1	10543	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	31898	PASS
199	198	5	9	6.2	1967	PASS
275	198	10	60	35.9	11465	PASS
365	198	1	100	5.4	1731	PASS
441	442	0.01	24	16.7	5164	PASS
442	198	50	100	96.7	30842	PASS
443	442	15	24	18.9	5815	PASS