


Data Path : Z:\HPCHEM1\BNA G\Data\BG020618\
 Data File : BG032578.D
 Acq On : 6 Feb 2018 23:26
 Operator : SJ/JU
 Sample : DFTPP
 Misc : MDL-W-8 ppm
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG012918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 06 18:57:08 2018

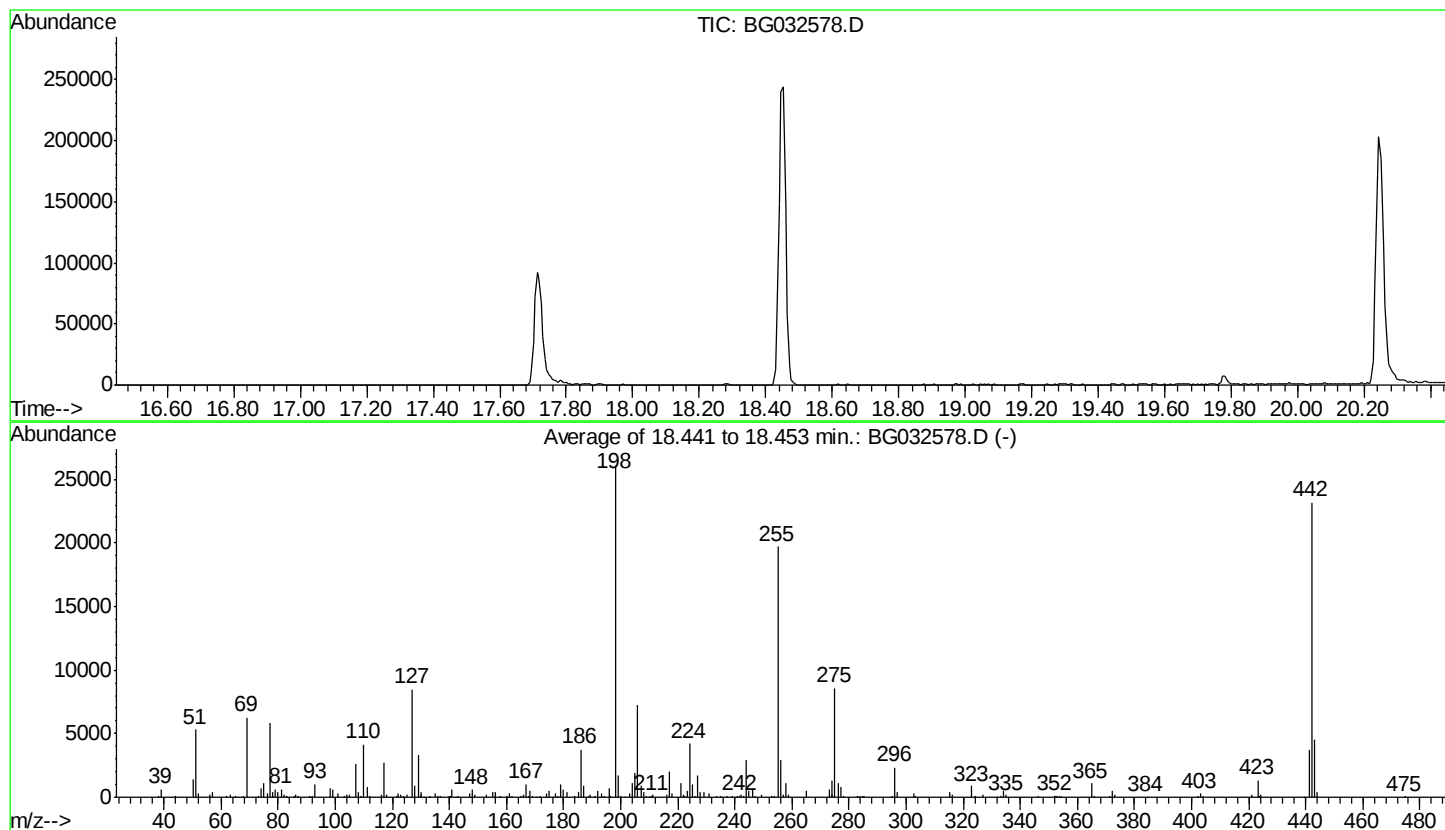

AutoFind: Scans 2579, 2580, 2581; Background Corrected with Scan 2573

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.3	5304	PASS
68	69	0.00	2	2.1	131	FAIL*
69	198	0.00	100	24.0	6258	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	32.5	8487	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	26077	PASS
199	198	5	9	6.6	1720	PASS
275	198	10	60	32.9	8569	PASS
365	198	1	100	4.1	1077	PASS
441	442	0.01	24	16.1	3727	PASS
442	198	50	100	88.9	23195	PASS
443	442	15	24	19.7	4572	PASS