
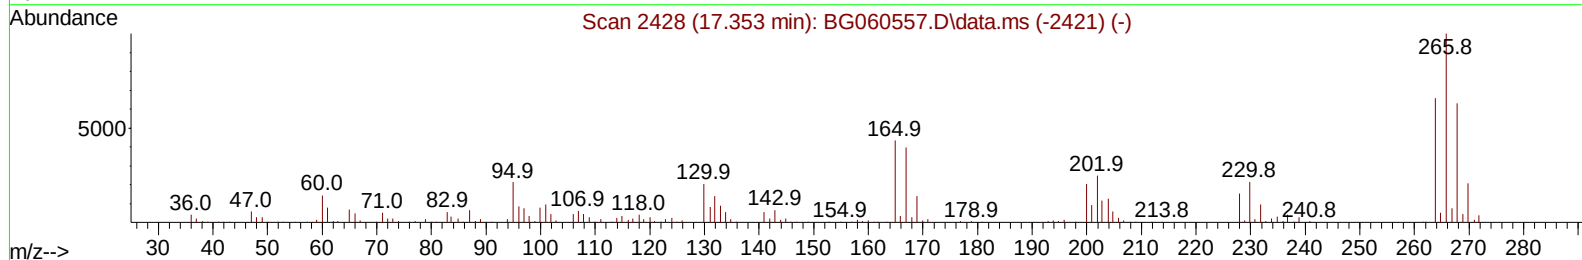
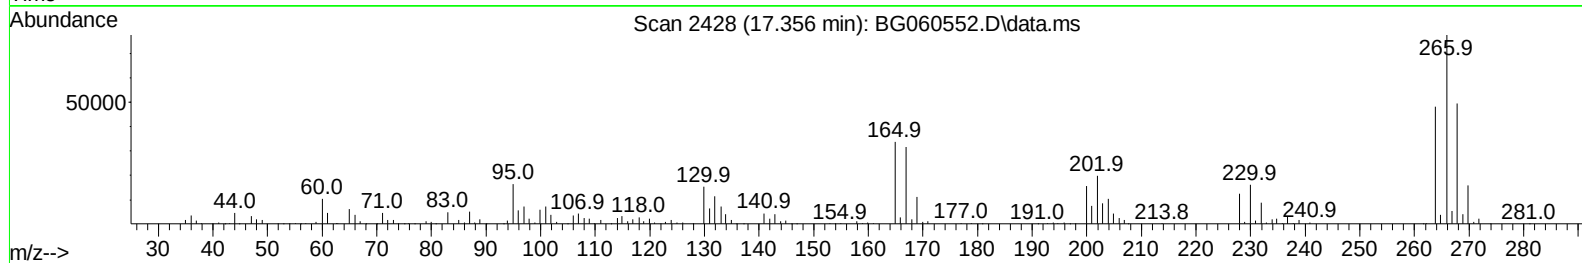


Quant Time: Feb 07 01:34:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : wed Feb 07 01:26:35 2024
Response via : Initial Calibration

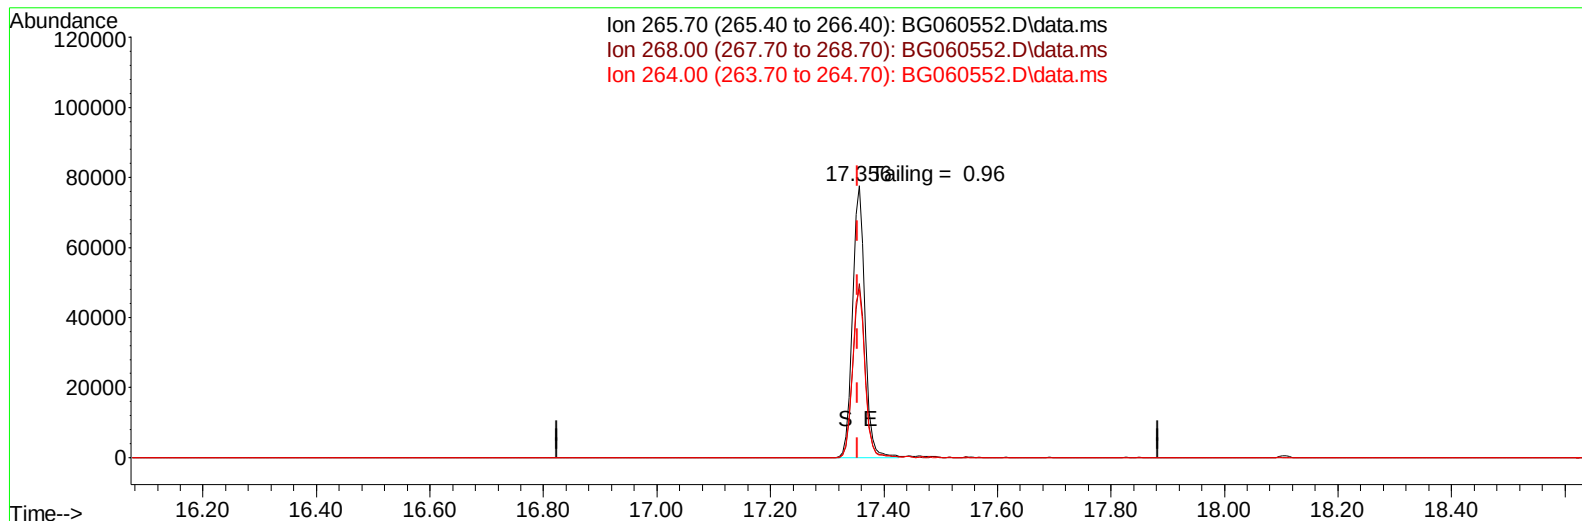




TIC: BG060552.D\data.ms

17.356min (+ 0.003) 27551.53 ng m

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.97
264.00	65.90	61.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020624\
Data File : BG060552.D
Acq On : 6 Feb 2024 9:52
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 07 01:34:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 07 01:26:35 2024
Response via : Initial Calibration

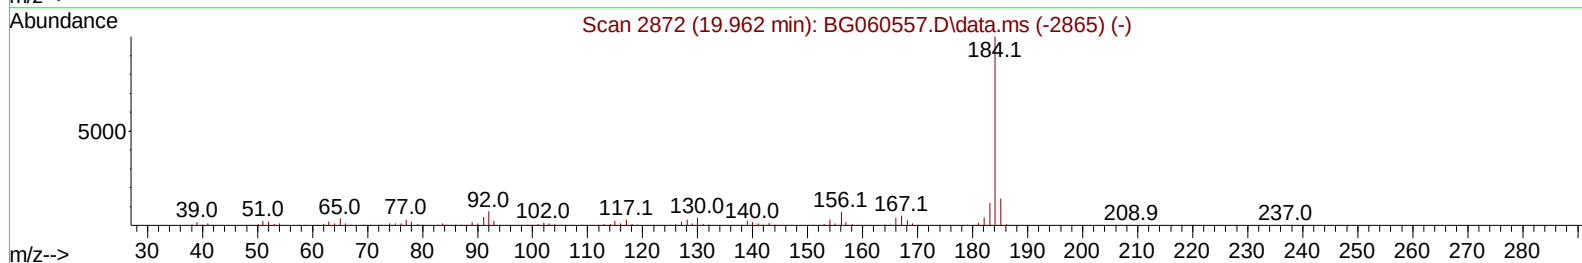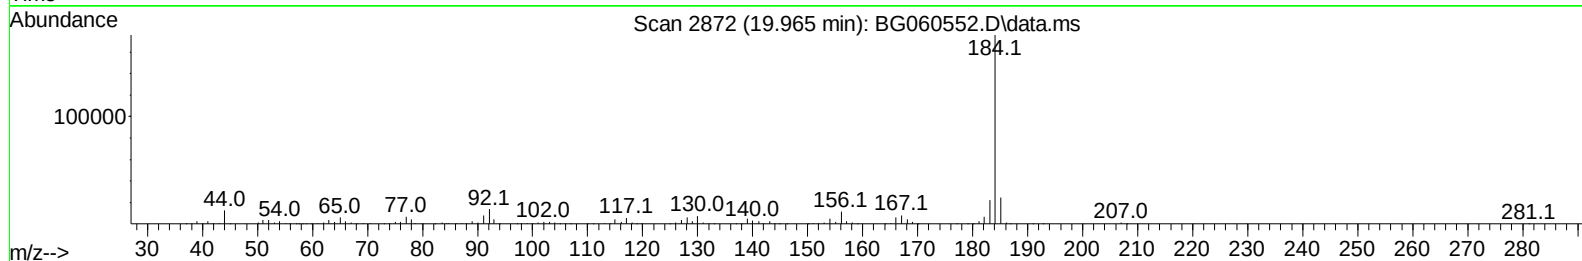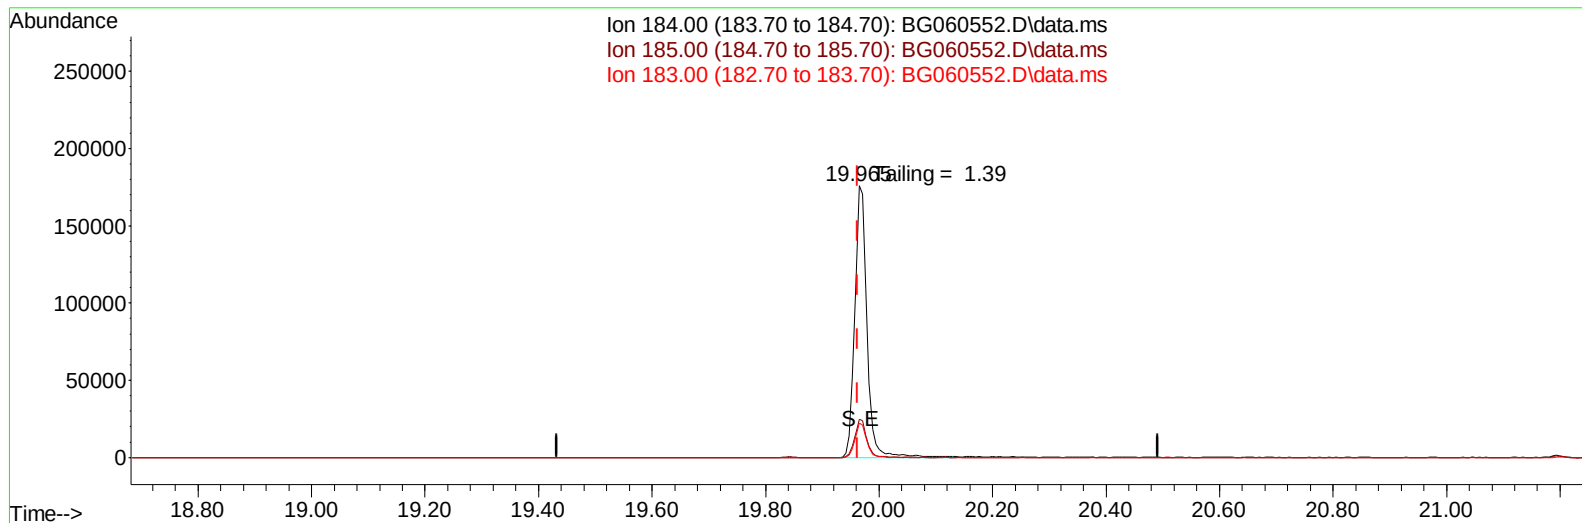

TIC: BG060552.D\data.ms

(77) Benzidine**19.965min (+ 0.003) 0.00 ng****response 265504**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.09
183.00	11.70	12.54
0.00	0.00	0.00