
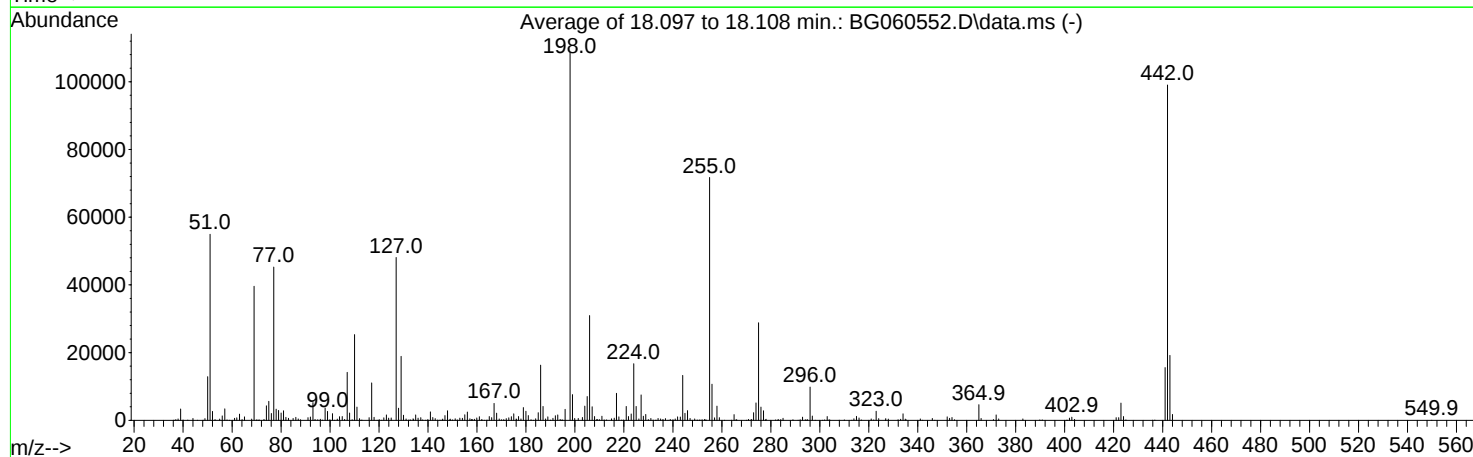


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020624\
Data File : BG060552.D
Acq On : 6 Feb 2024 9:52
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Feb 07 01:26:35 2024

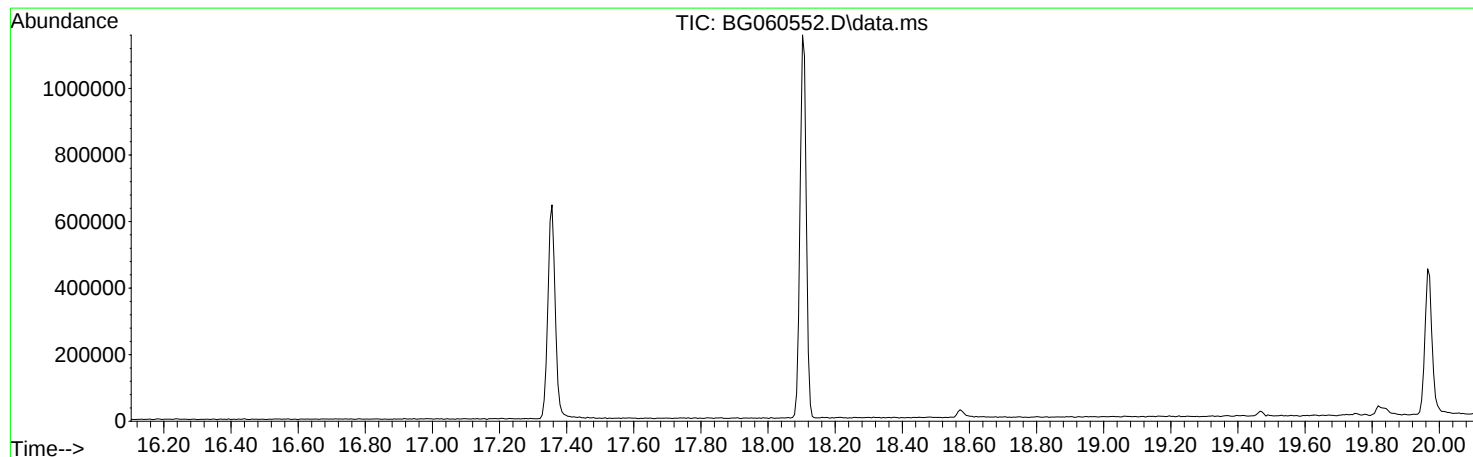




AutoFind: Scans 2554, 2555, 2556; Background Corrected with Scan 2548

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.6	54936	PASS
68	69	0.00	2	1.0	392	PASS
69	198	0.00	100	36.4	39577	PASS
70	69	0.00	2	0.4	139	PASS
127	198	10	80	44.3	48088	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	108635	PASS
199	198	5	9	7.0	7613	PASS
275	198	10	60	26.6	28845	PASS
365	198	1	100	4.3	4644	PASS
441	198	0.01	100	14.3	15580	PASS
442	442	50	100	100.0	99059	PASS
443	442	15	24	19.4	19196	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020624\
Data File : BG060552.D
Acq On : 6 Feb 2024 9:52
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 07 01:34:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 07 01:26:35 2024
Response via : Initial Calibration

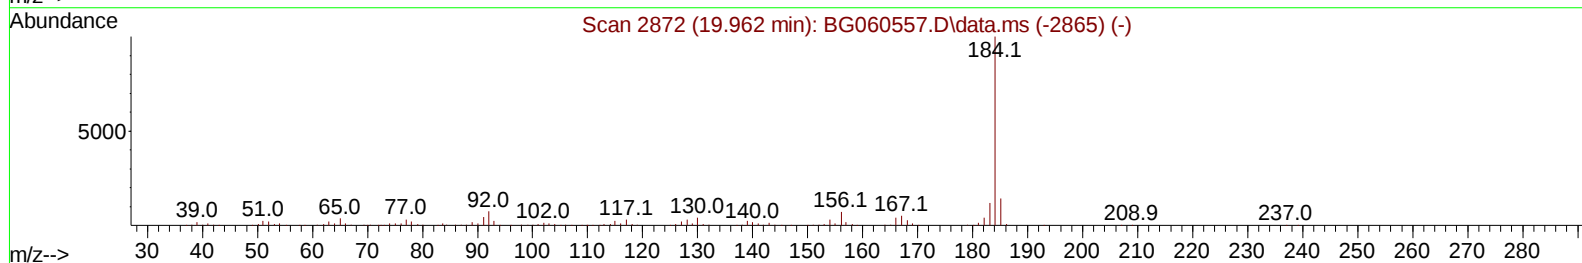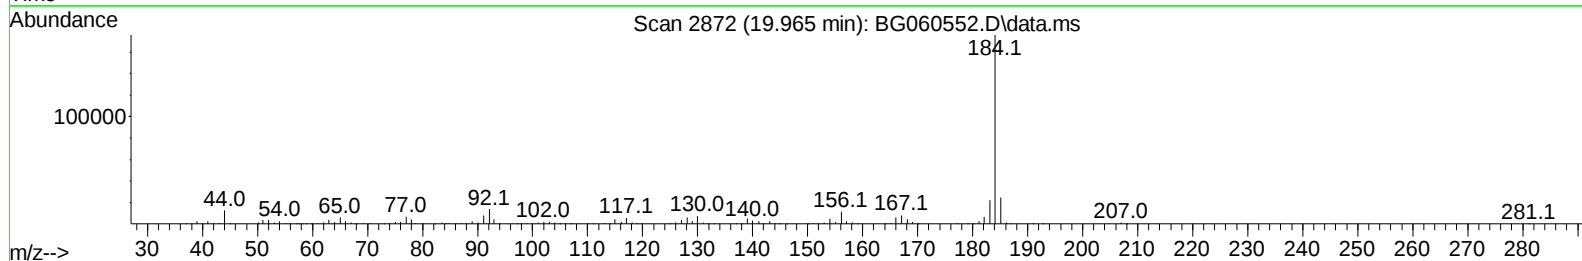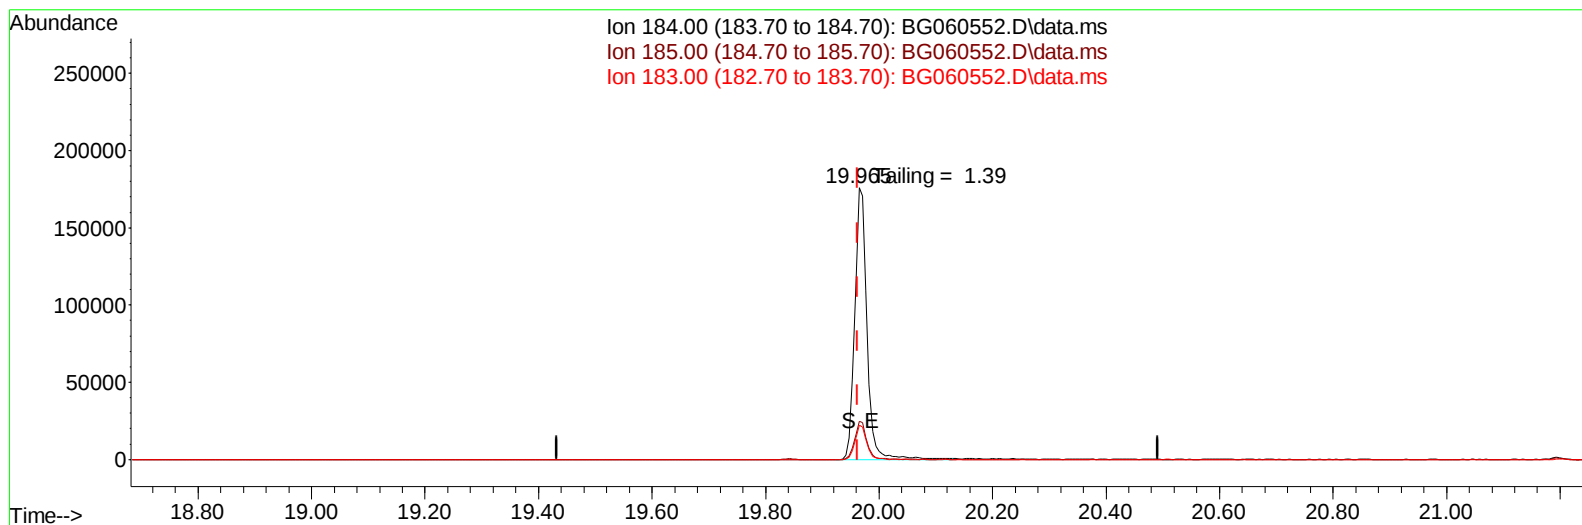

TIC: BG060552.D\data.ms

(77) Benzidine

19.965min (+ 0.003) 0.00 ng

response 265504

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.09
183.00	11.70	12.54
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/6/2024	BNA_G	<u>BG060552.D</u>
Compound Name	Response	Retention Time
DDT	250924	21.199
DDD	7363	20.729
DDE	208	20.224
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7571	258495	2.93

Instrument :
BNA_G
ClientSampleId :
DFTPP