
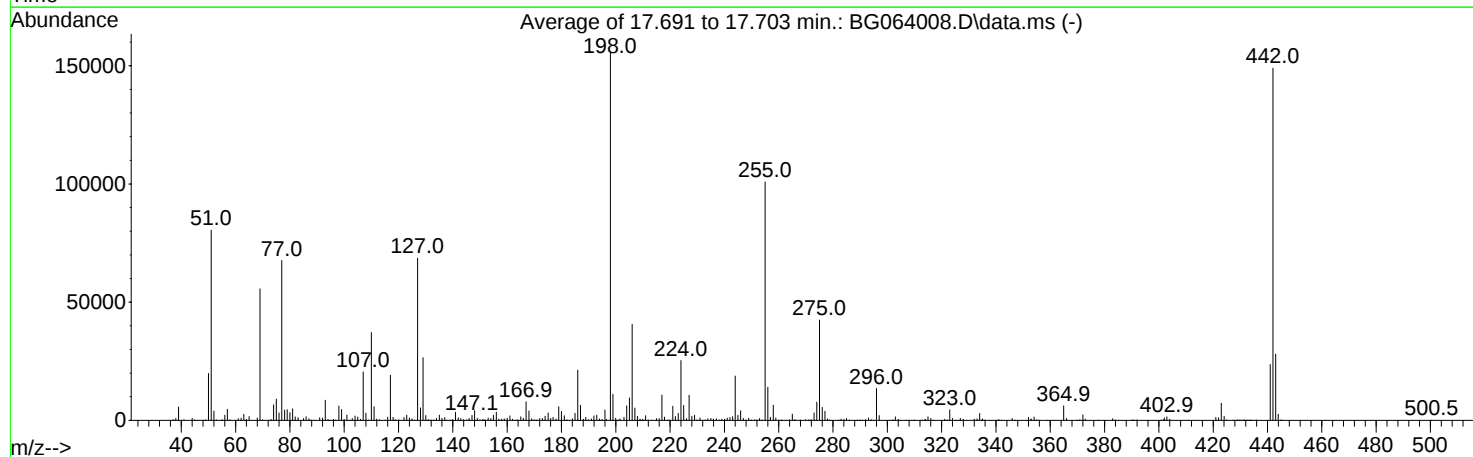


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020625\
Data File : BG064008.D
Acq On : 6 Feb 2025 9:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Feb 04 02:51:00 2025

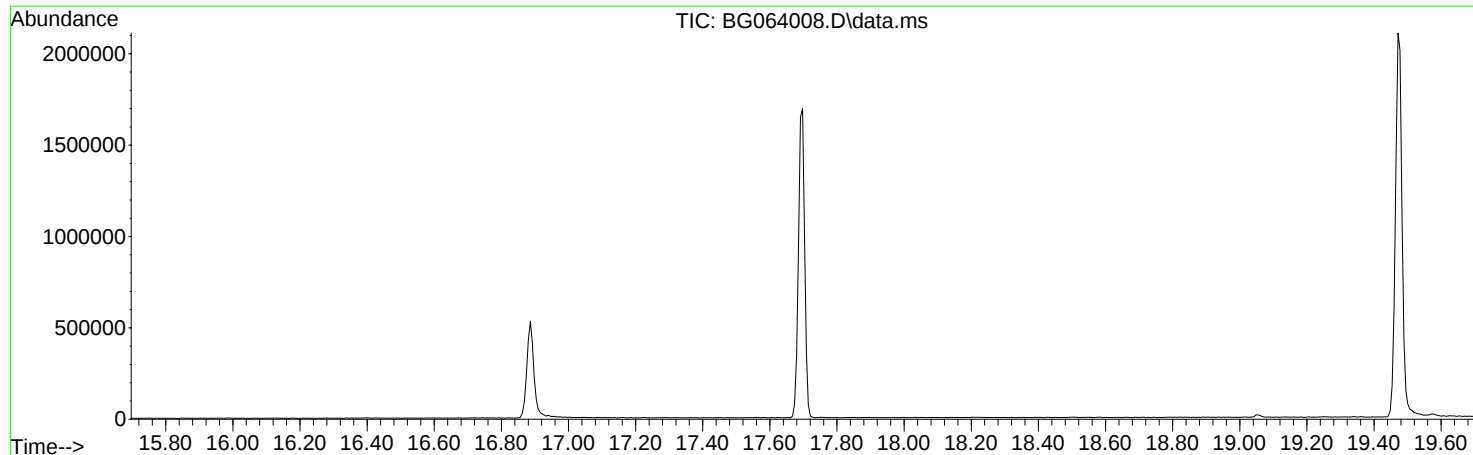

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2477

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.7	80517	PASS
68	69	0.00	2	1.9	1031	PASS
69	198	0.00	100	35.7	55629	PASS
70	69	0.00	2	0.5	273	PASS
127	198	10	80	44.1	68659	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	155616	PASS
199	198	5	9	7.1	11020	PASS
275	198	10	60	27.3	42459	PASS
365	198	1	100	4.0	6164	PASS
441	198	0.01	100	15.2	23653	PASS
442	442	50	100	100.0	148971	PASS
443	442	15	24	18.8	28037	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/6/2025	BNA_G	<u>BG064008.D</u>
Compound Name	Response	Retention Time
DDT	365957	20.711
DDD	12965	20.271
DDE	242	19.771
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13207	379164	3.48

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020625\
Data File : BG064008.D
Acq On : 6 Feb 2025 9:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 06 09:41:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 04 02:51:00 2025
Response via : Initial Calibration

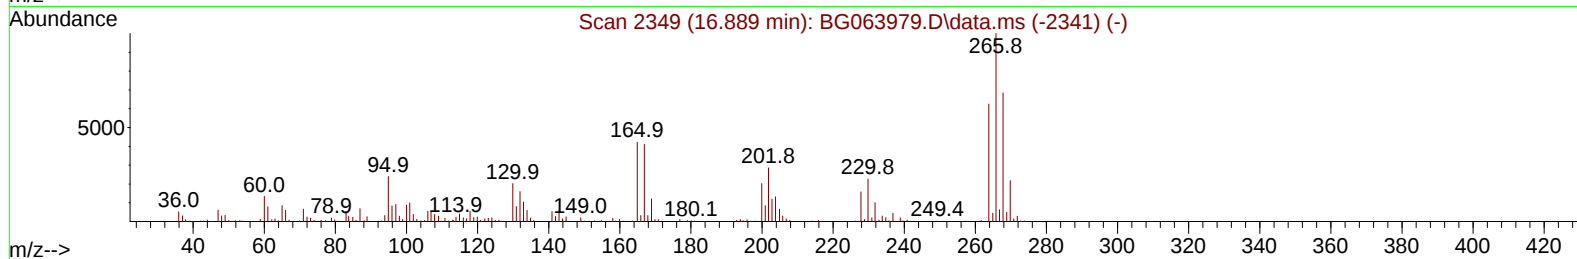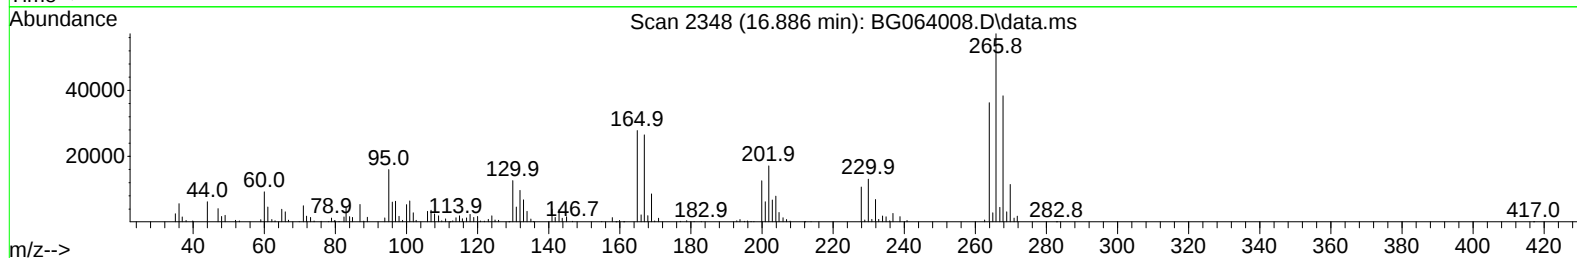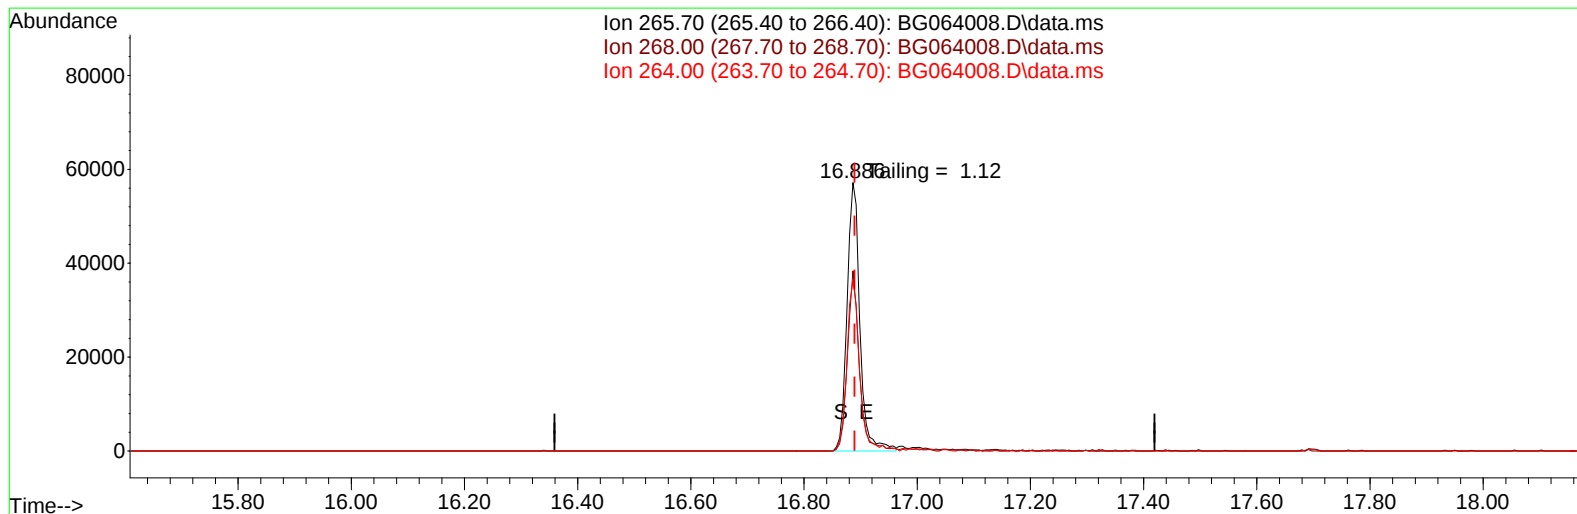

TIC: BG064008.D\data.ms

(70) Pentachlorophenol (C)

16.886min (-0.003) 12561.18 ng




response 90224

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.50	67.10
264.00	62.50	63.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020625\
Data File : BG064008.D
Acq On : 6 Feb 2025 9:03
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 06 09:41:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 04 02:51:00 2025
Response via : Initial Calibration

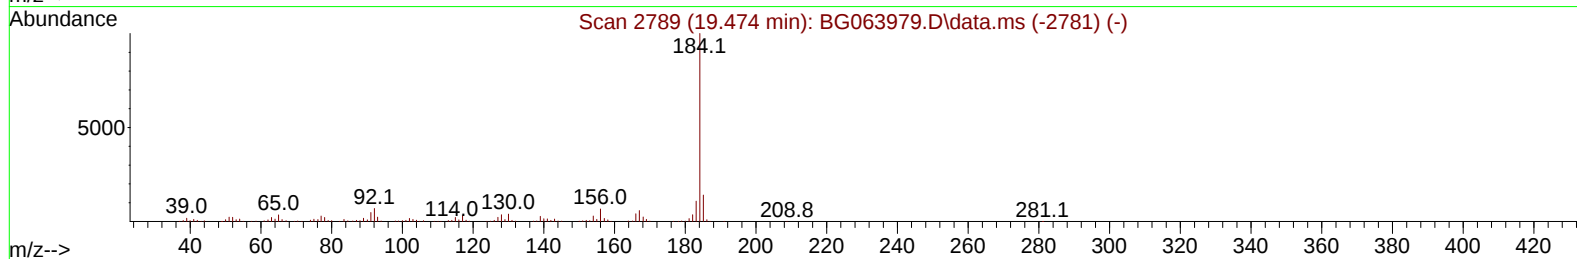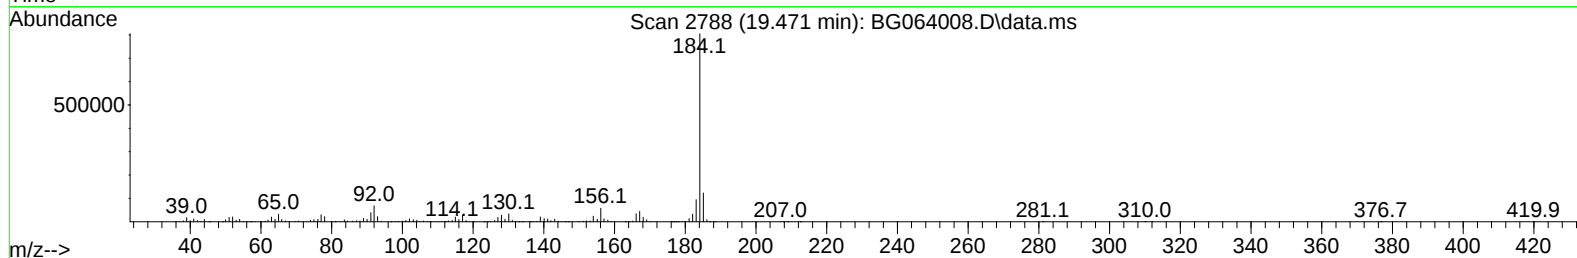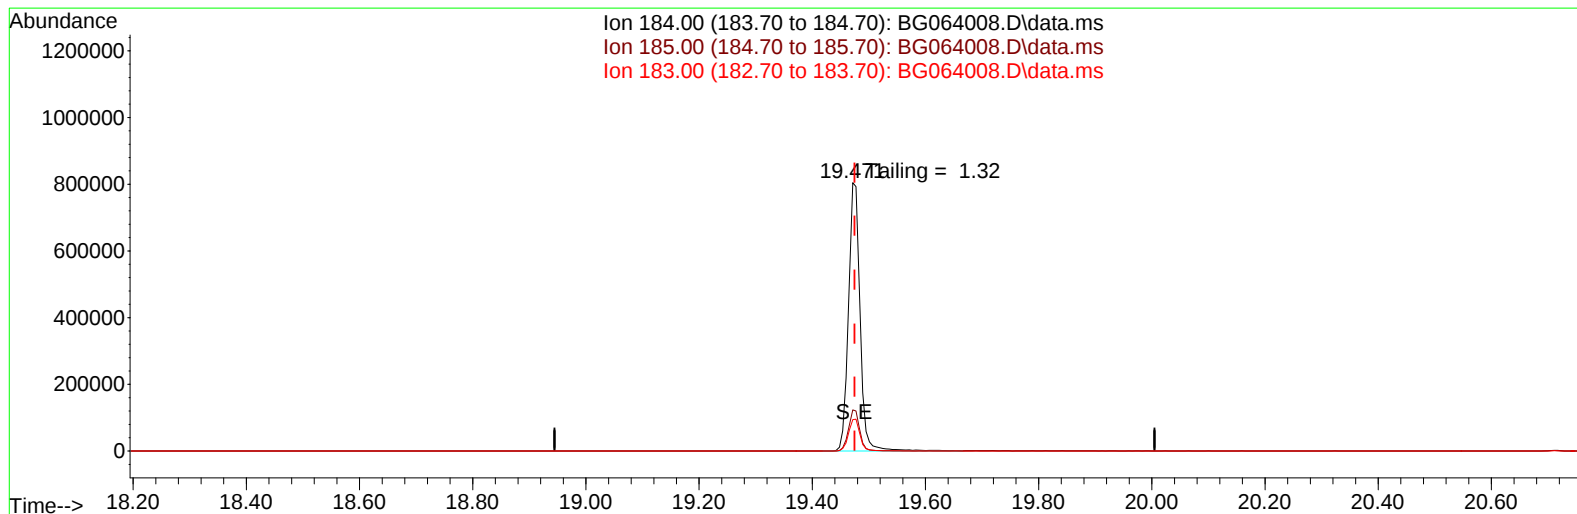

TIC: BG064008.D\data.ms

(77) Benzidine

19.471min (-0.003) 0.00 ng

response 1145328

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	15.33
183.00	10.90	11.73
0.00	0.00	0.00