
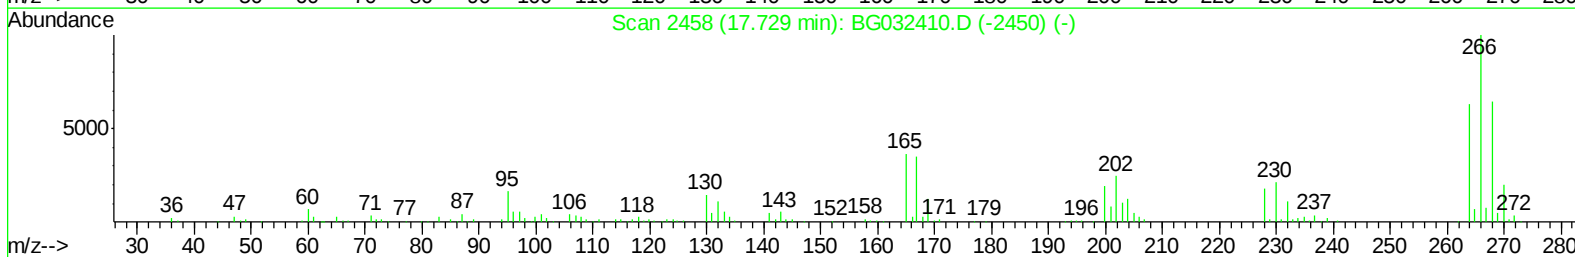
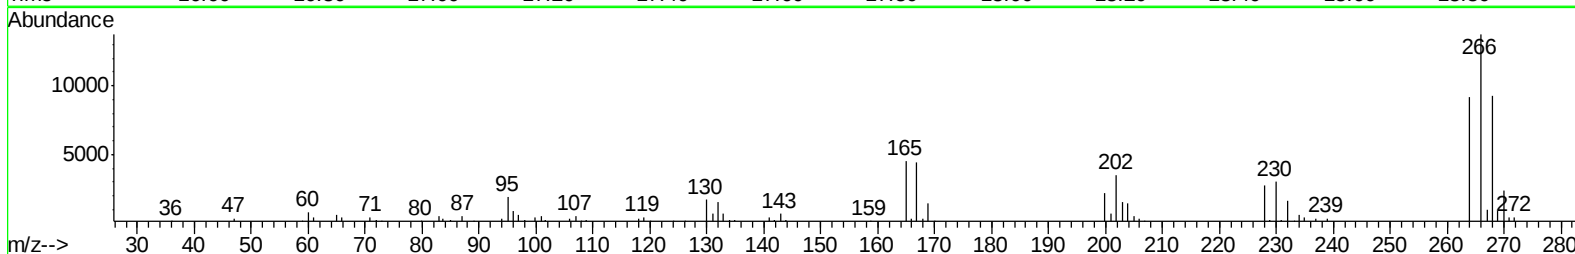


Data Path : Z:\HPCHEM1\BNA G\DATA\BG020718\
Data File : BG032593.D
Acq On : 7 Feb 2018 13:22
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 04:06:14 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 18:57:08 2018
Response via : Initial Calibration

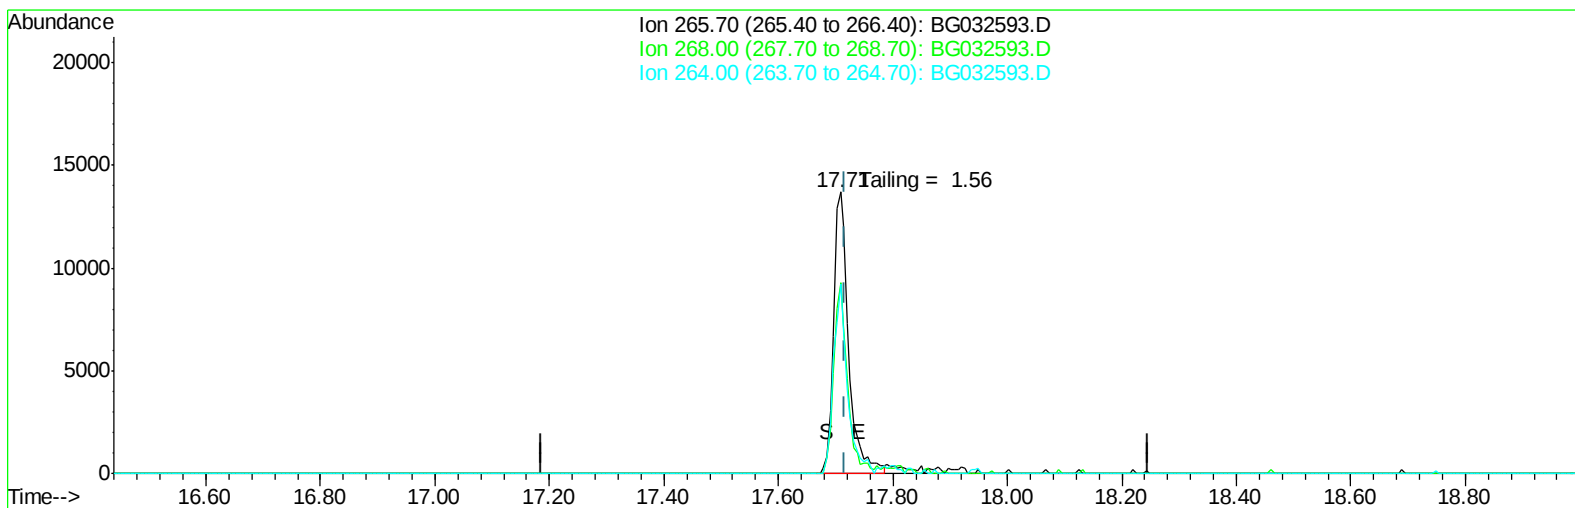

TIC: BG032593.D

(69) Pentachlorophenol (C)




17.708min (-0.009) 43286.58ng

response 24896

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	67.83
264.00	62.00	67.09
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG020718\
 Data File : BG032593.D
 Acq On : 7 Feb 2018 13:22
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 04:06:14 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 06 18:57:08 2018
 Response via : Initial Calibration

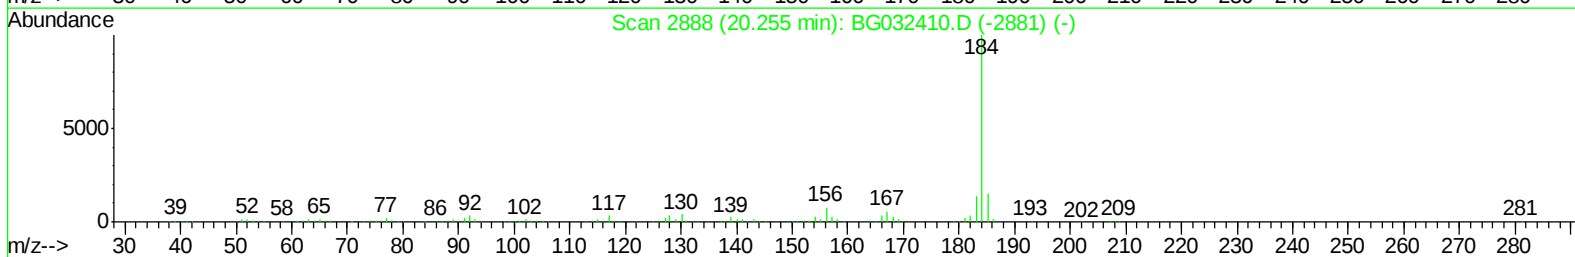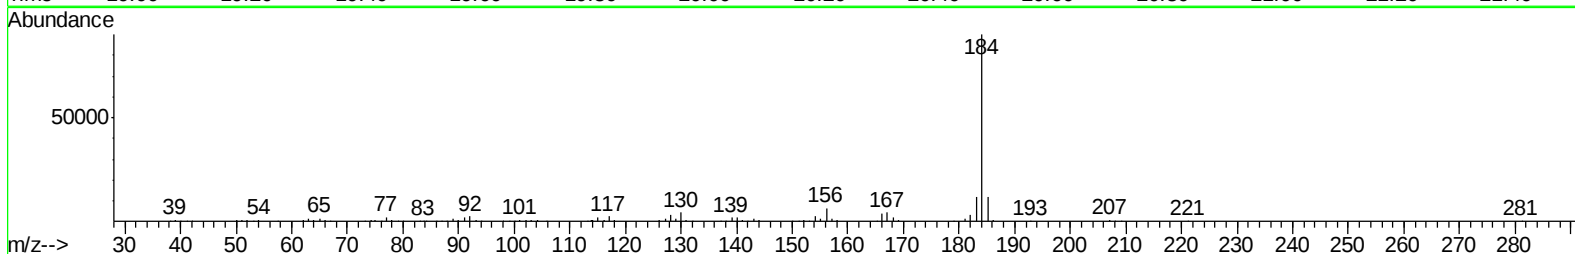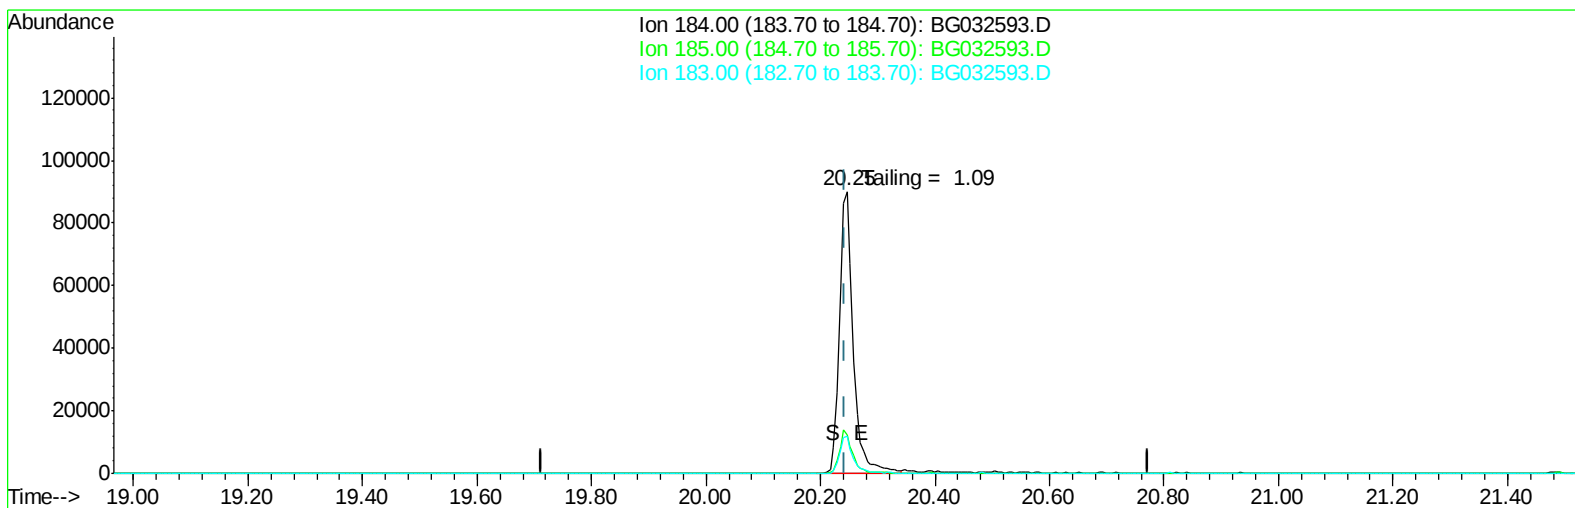

TIC: BG032593.D

(76) Benzidine

20.246min (+0.003) 0.00ng

response 152439

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.47
183.00	13.30	13.09
0.00	0.00	0.00