
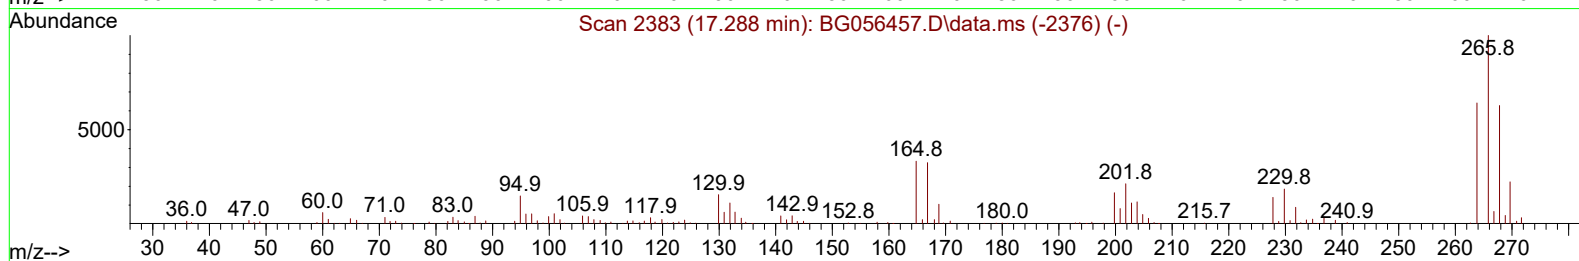
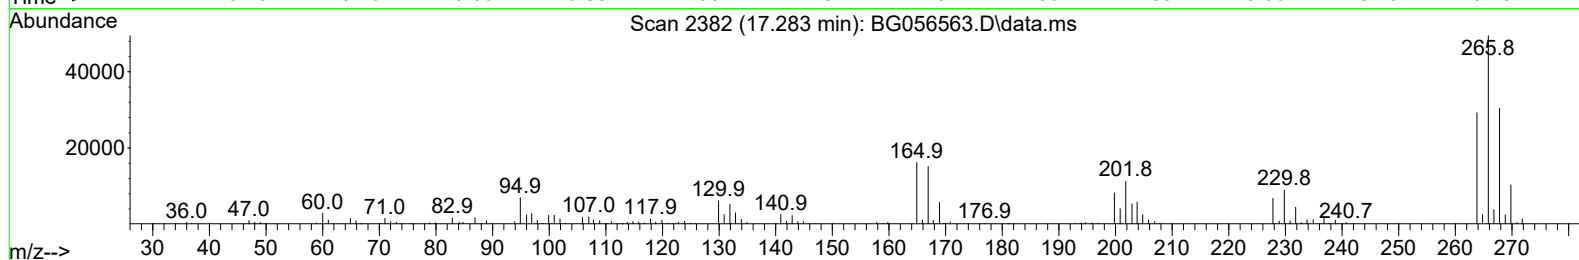


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020723\
Data File : BG056563.D
Acq On : 7 Feb 2023 11:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 05:12:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 08 03:02:11 2023
Response via : Initial Calibration

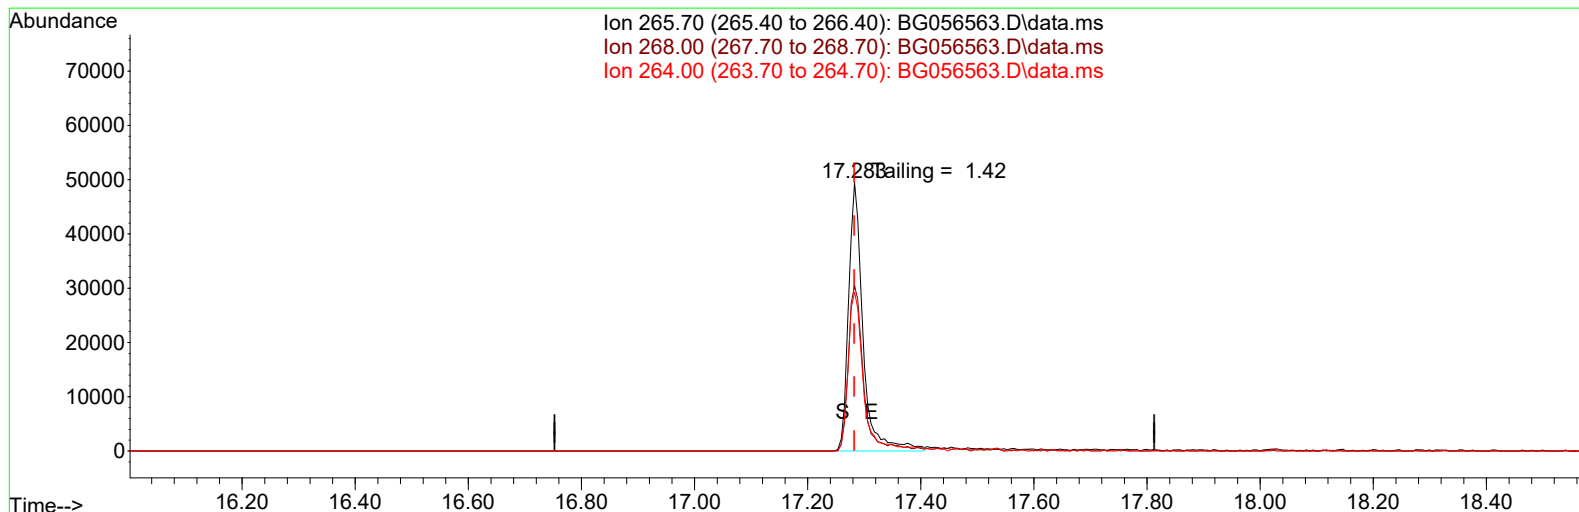

TIC: BG056563.D\data.ms

(70) Pentachlorophenol (C)




17.283min (+ 0.000) 20611.66 ng

response 86163

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	61.57
264.00	64.20	59.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020723\
Data File : BG056563.D
Acq On : 7 Feb 2023 11:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 08 05:12:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 08 03:02:11 2023
Response via : Initial Calibration

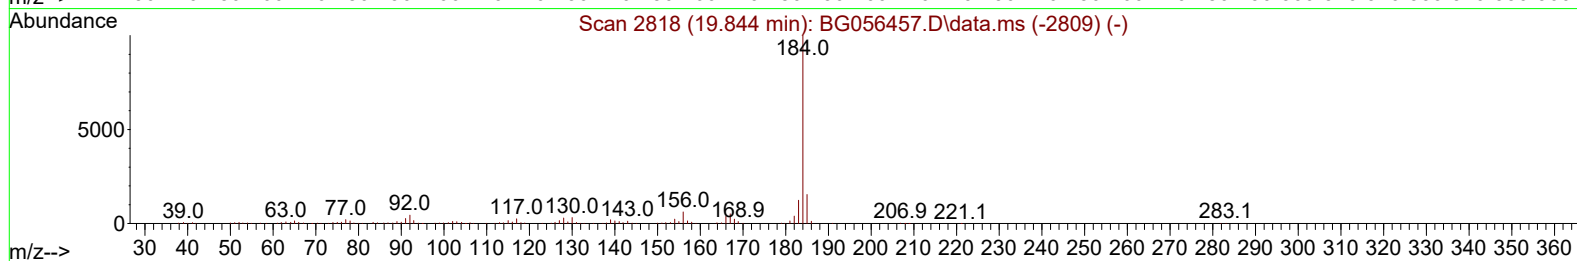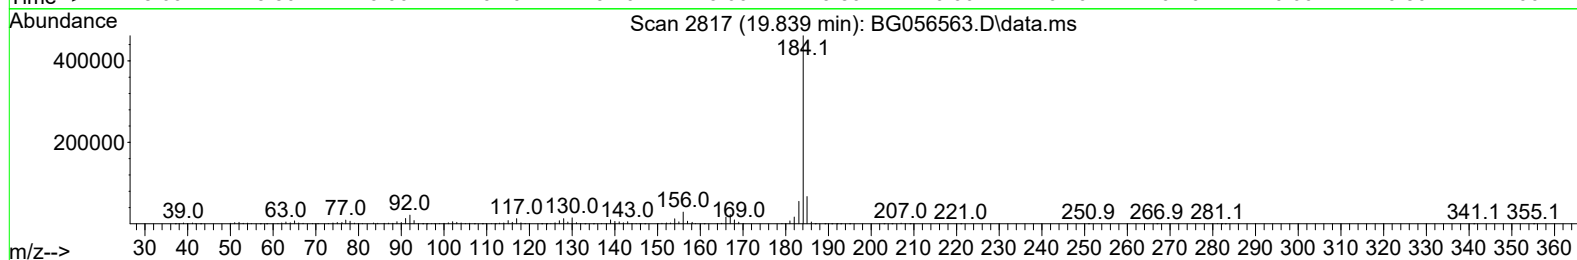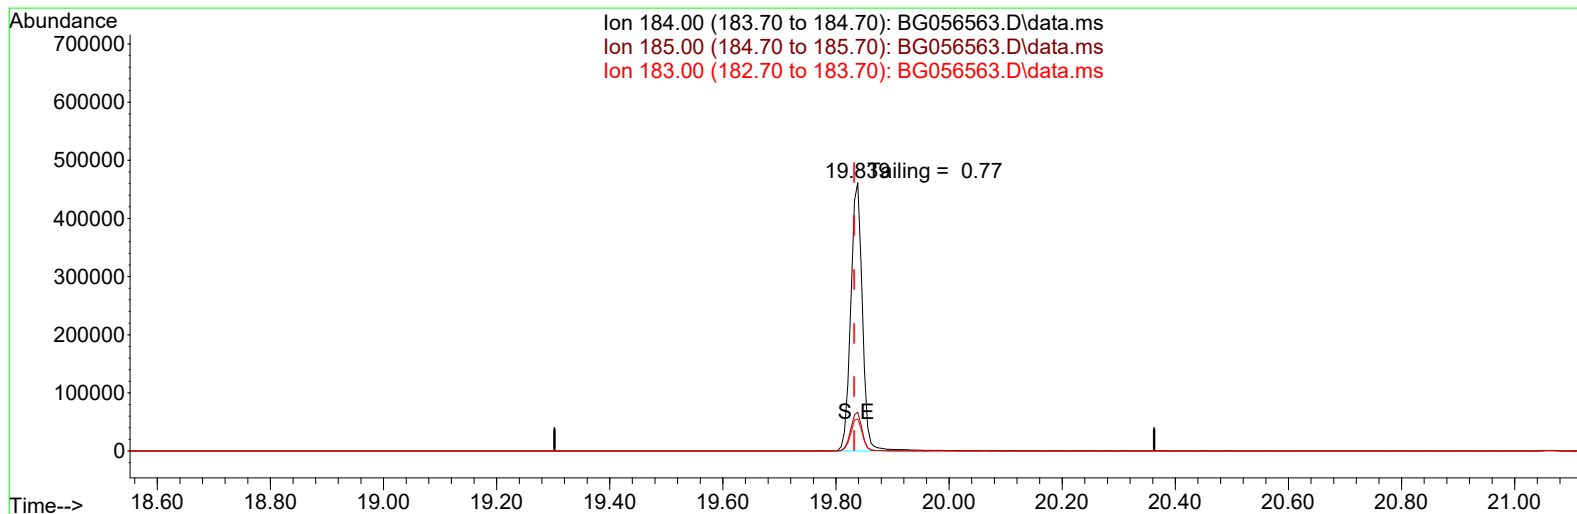

TIC: BG056563.D\data.ms

(77) Benzidine**19.839min (+ 0.006) 208690.87 ng****response 660749**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.52
183.00	12.30	11.95
0.00	0.00	0.00