


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020723\
 Data File : BG056563.D
 Acq On : 7 Feb 2023 11:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 08 03:02:11 2023

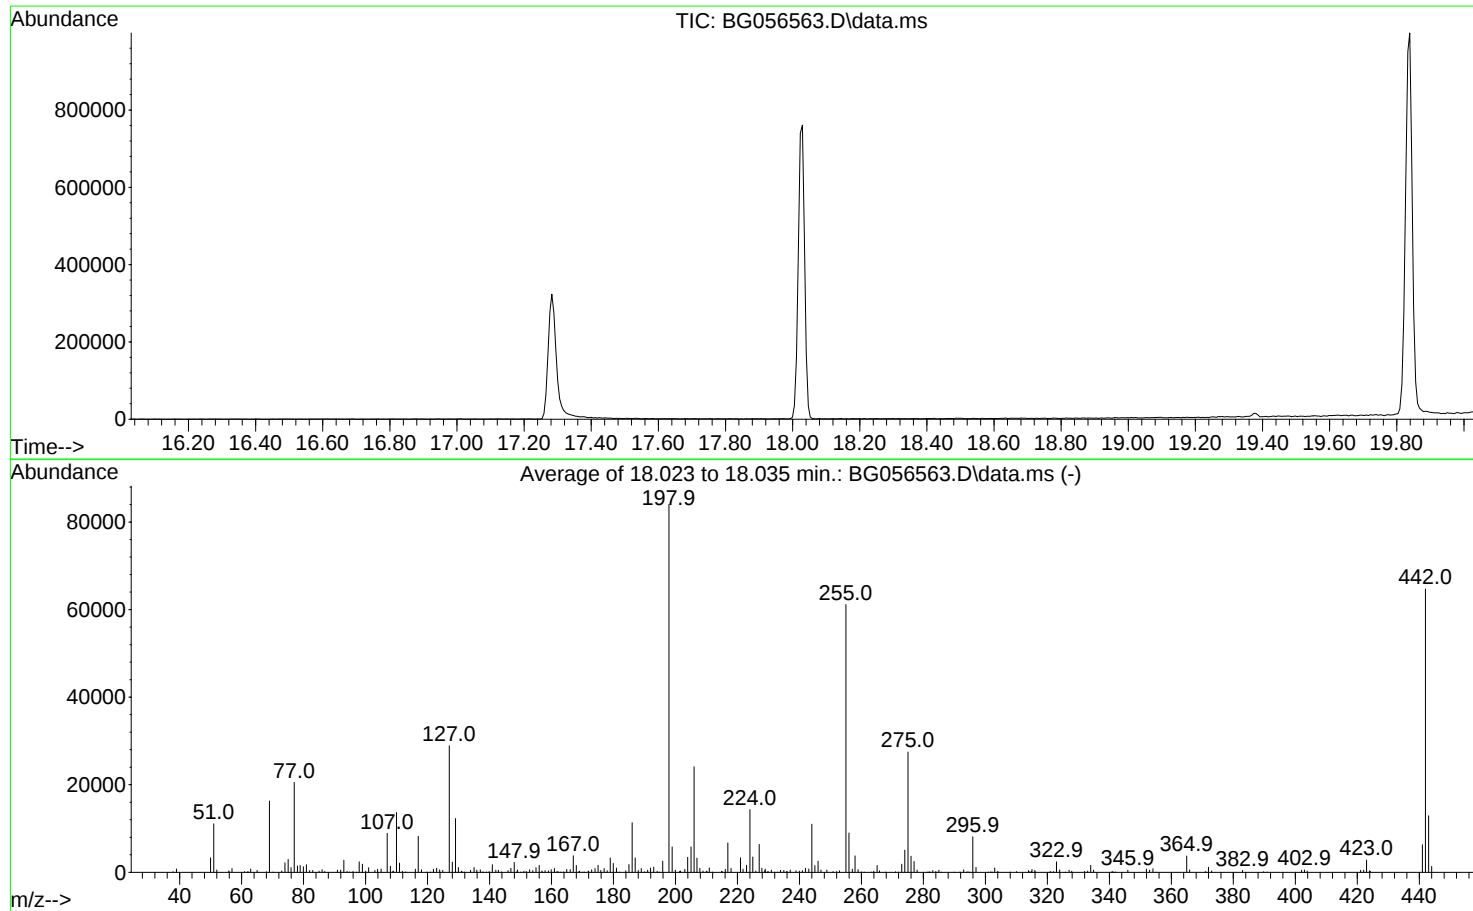




AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	13.1	11042	PASS
68	69	0.00	2	0.8	132	PASS
69	198	0.00	100	19.4	16302	PASS
70	69	0.00	2	0.4	70	PASS
127	198	10	80	34.4	28883	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	84024	PASS
199	198	5	9	6.9	5789	PASS
275	198	10	60	32.7	27475	PASS
365	198	1	100	4.4	3713	PASS
441	198	0.01	100	7.5	6293	PASS
442	442	50	100	100.0	64720	PASS
443	442	15	24	19.9	12910	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020723\
Data File : BG056563.D
Acq On : 7 Feb 2023 11:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 08 05:12:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 08 03:02:11 2023
Response via : Initial Calibration

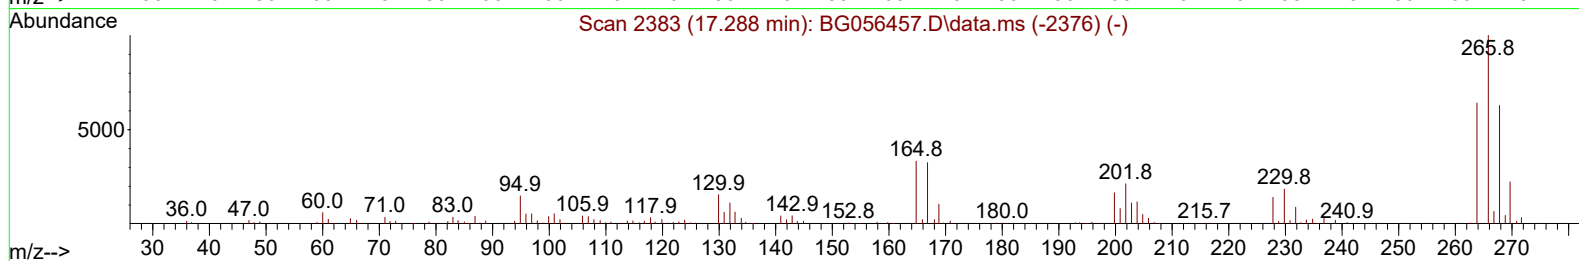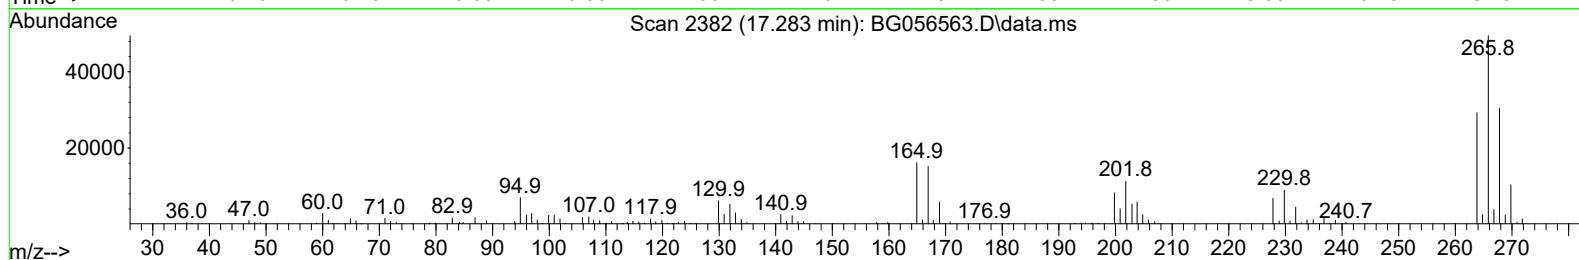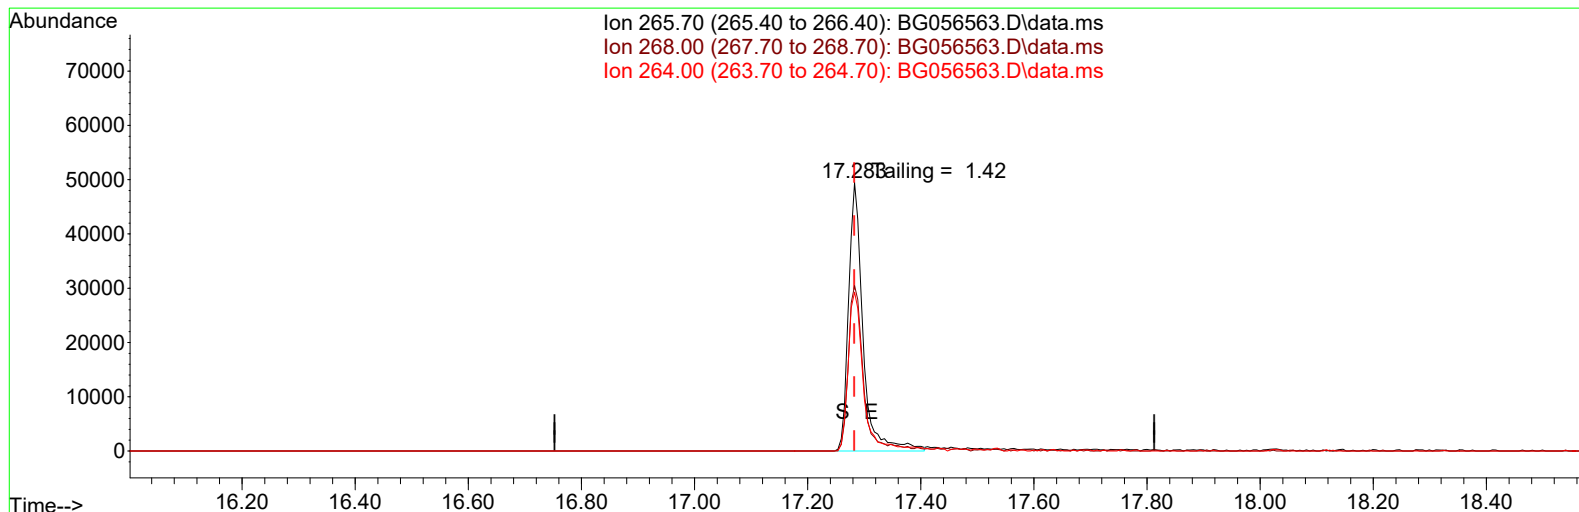

TIC: BG056563.D\data.ms

(70) Pentachlorophenol (C)

17.283min (+ 0.000) 20611.66 ng




response 86163

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	61.57
264.00	64.20	59.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020723\
Data File : BG056563.D
Acq On : 7 Feb 2023 11:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 08 05:12:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 08 03:02:11 2023
Response via : Initial Calibration

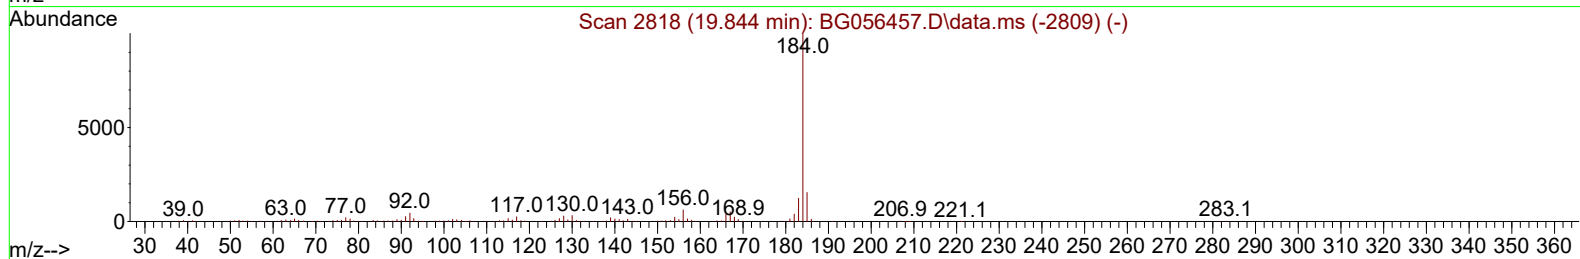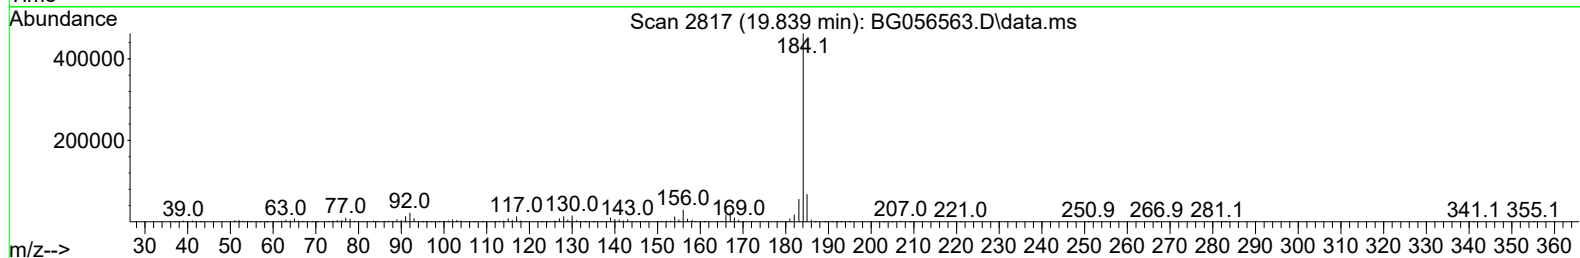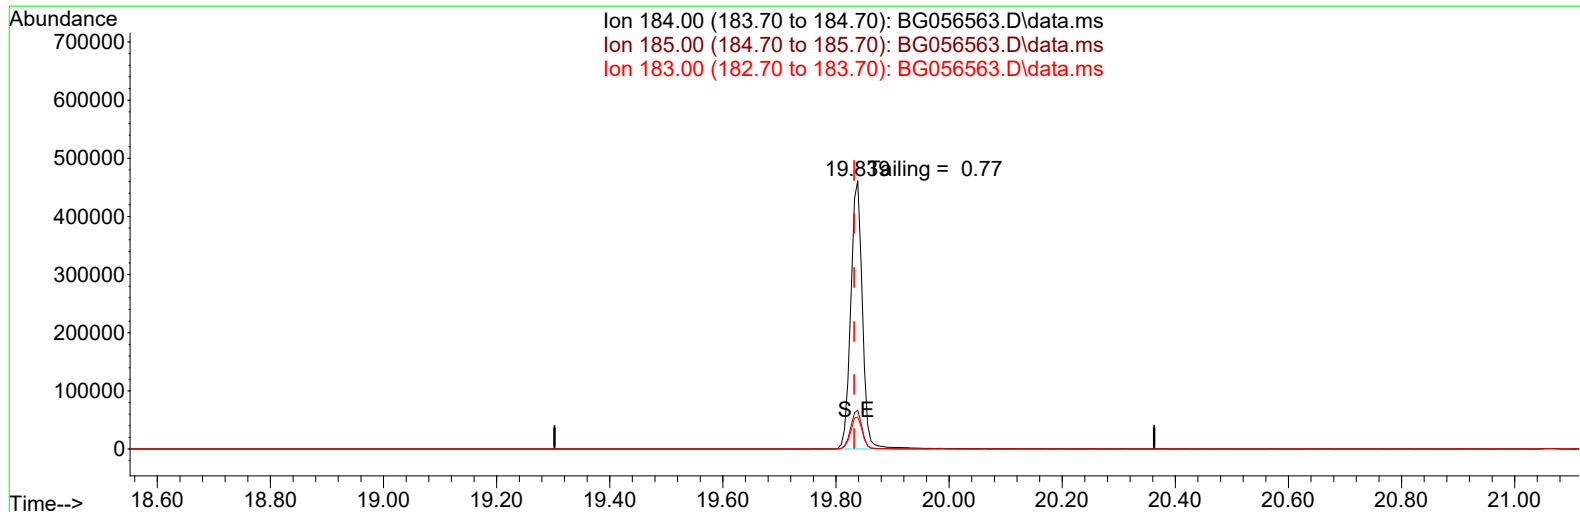

TIC: BG056563.D\data.ms

(77) Benzidine

19.839min (+ 0.006) 208690.87 ng

response 660749

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.52
183.00	12.30	11.95
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/7/2023	BNA_G	BG056563.D
Compound Name	Response	Retention Time
DDT	299118	21.066
DDD	10521	20.614
DDE	918	20.199
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11439	310557	3.68

Instrument :
BNA_G
ClientSampleId :
DFTPP