


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG020816\
 Data File : BG020804.D
 Acq On : 8 Feb 2016 10:59
 Operator : SJ/UM
 Sample : DFTPP29
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP29

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG020816.M
 Title : SVOA CALIBRATION
 Last Update : Tue Feb 09 05:03:11 2016

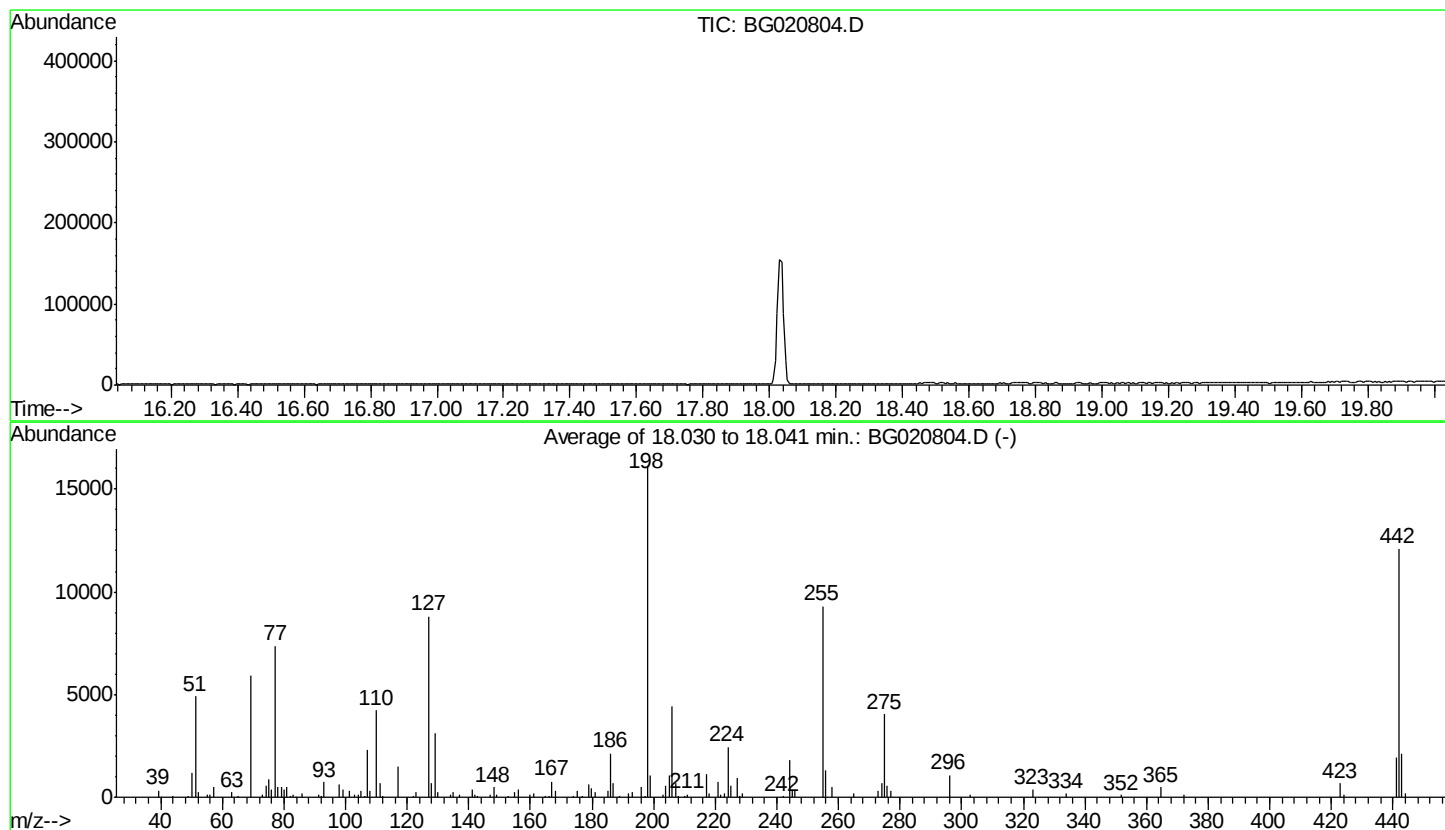

AutoFind: Scans 2586, 2587, 2588; Background Corrected with Scan 2581

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	4916	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.6	5901	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.6	8817	PASS
197	198	0.00	2	0.4	57	PASS
198	198	100	100	100.0	16143	PASS
199	198	5	9	6.5	1057	PASS
275	198	10	60	25.0	4028	PASS
365	198	1	100	3.0	486	PASS
441	442	0.01	100	15.9	1924	PASS
442	198	50	100	75.0	12113	PASS
443	442	15	24	17.7	2143	PASS

m/z	Abundance
39.15	396.0
40.05	196.0
44.05	271.0
49.05	347.0
50.05	1536.0
51.15	6496.0
52.05	270.0
55.05	150.0
56.05	275.0
57.05	640.0
63.05	297.0
65.05	206.0
69.05	7740.0
73.05	156.0
74.05	666.0
75.05	1136.0
76.05	492.0
77.15	9683.0
78.15	575.0
79.05	540.0
80.05	497.0
81.05	569.0
82.05	161.0
82.95	212.0
84.05	378.0
86.05	407.0
91.05	217.0
92.05	188.0
93.05	842.0
98.05	819.0
99.05	478.0
101.05	283.0
103.05	165.0
104.05	251.0
105.05	377.0
107.05	2925.0
107.95	368.0
110.05	5004.0
111.05	870.0
112.05	159.0
117.05	1802.0
121.95	268.0
123.05	250.0
127.05	11062.0
128.05	875.0
129.05	3756.0
129.95	327.0
133.95	188.0
134.95	333.0
136.95	174.0
140.95	495.0
141.95	150.0
142.95	163.0
146.95	240.0
147.95	616.0
148.95	171.0
155.05	360.0
155.95	478.0
159.95	185.0
160.95	286.0
164.95	203.0
165.95	171.0
167.05	931.0
167.95	414.0
175.05	423.0
177.05	237.0
178.95	741.0
179.95	469.0
180.95	278.0
185.05	357.0
186.05	2591.0
187.05	727.0
191.95	227.0
193.05	270.0
195.95	496.0
197.95	18880.0
198.95	1419.0
202.85	198.0
203.95	643.0
204.95	1192.0
206.05	5059.0
207.05	796.0
207.95	206.0
211.05	170.0
216.95	1240.0
217.95	174.0
220.95	785.0
221.85	162.0
222.95	278.0
224.05	2892.0
224.95	605.0

Instrument :
BNA_G
ClientSampleId :
DFTPP29

226.95	1080.0
228.95	225.0
241.95	164.0
243.95	2139.0
244.95	413.0
245.95	327.0
254.95	10433.0
255.95	1476.0
257.95	601.0
264.95	260.0
272.95	354.0
273.95	774.0
274.95	4519.0
275.95	565.0
276.95	352.0
295.95	1100.0
302.95	152.0
322.95	310.0
333.95	284.0
351.95	170.0
364.85	605.0
371.95	180.0
422.85	585.0
423.95	155.0
440.95	1768.0
441.95	11315.0
442.95	2048.0
443.85	205.0

Instrument :
BNA_G
ClientSampleId :
DFTPP29

m/z	Abundance
39.05	356.0
40.05	184.0
44.05	274.0
49.05	295.0
50.15	1240.0
51.15	5350.0
52.05	237.0
56.05	197.0
57.05	457.0
63.15	217.0
69.05	6405.0
73.05	181.0
74.15	687.0
75.05	972.0
76.05	384.0
77.15	8203.0
78.15	620.0
79.05	558.0
80.05	344.0
81.05	564.0
83.05	187.0
83.95	344.0
85.95	329.0
91.05	192.0
93.05	799.0
98.05	694.0
99.05	499.0
101.05	388.0
103.05	196.0
103.95	171.0
105.05	383.0
106.05	154.0
107.05	2579.0
108.05	413.0
110.05	5000.0
111.05	778.0
117.05	1861.0
122.95	327.0
127.05	9942.0
127.95	730.0
129.05	3706.0
130.05	415.0
133.95	159.0
134.95	238.0
137.05	179.0
140.95	384.0
142.05	185.0
147.05	202.0
148.05	521.0
149.05	160.0
152.95	162.0
154.95	275.0
155.95	380.0
160.05	179.0
160.95	235.0
167.05	927.0
168.05	330.0
174.05	161.0
175.05	326.0
178.95	618.0
179.95	511.0
180.95	236.0
184.95	414.0
186.05	2347.0
186.95	737.0
188.95	159.0
192.05	213.0
192.95	253.0
195.95	588.0
197.95	19040.0
198.95	1145.0
202.95	163.0
203.95	676.0
204.95	1302.0
206.05	5200.0
206.95	750.0
209.95	155.0
211.05	224.0
216.95	1350.0
217.95	174.0
220.95	889.0
221.65	236.0
222.95	320.0
224.05	2866.0
224.95	688.0
226.95	1101.0
227.95	187.0
228.95	234.0
244.05	2062.0
244.95	331.0
245.95	363.0

Instrument :
BNA_G
ClientSampleId :
DFTPP29

254.95	10721.0
255.95	1567.0
257.95	509.0
264.95	234.0
272.95	324.0
273.95	787.0
274.95	4750.0
275.95	604.0
276.95	314.0
295.95	1229.0
302.95	163.0
322.95	456.0
333.95	227.0
351.95	176.0
364.85	526.0
371.95	182.0
422.95	779.0
423.95	155.0
440.95	2285.0
441.95	14173.0
442.95	2479.0
443.95	238.0

Instrument :
BNA_G
ClientSampleId :
DFTPP29

m/z	Abundance
39.15	233.0
40.05	183.0
43.15	214.0
44.05	284.0
49.05	232.0
50.05	746.0
51.15	2904.0
52.05	180.0
55.05	176.0
57.15	338.0
63.05	194.0
69.05	3559.0
74.05	349.0
75.05	552.0
76.05	288.0
77.05	4263.0
78.05	304.0
79.05	372.0
79.95	198.0
81.05	340.0
84.05	323.0
85.95	250.0
93.05	522.0
98.05	385.0
99.05	241.0
101.05	215.0
105.05	235.0
107.05	1444.0
108.05	223.0
110.05	2642.0
111.05	417.0
117.05	912.0
123.05	189.0
127.05	5448.0
128.05	390.0
129.05	1940.0
135.05	163.0
140.95	328.0
147.95	308.0
154.95	176.0
156.05	223.0
166.95	454.0
167.95	247.0
175.05	183.0
178.95	492.0
179.95	331.0
180.95	173.0
184.95	187.0
185.95	1474.0
186.95	538.0
191.85	152.0
192.95	197.0
195.95	474.0
197.05	172.0
197.95	10511.0
198.95	609.0
203.95	402.0
204.95	628.0
206.05	3029.0
206.95	440.0
216.95	765.0
217.85	154.0
220.85	504.0
224.05	1541.0
224.95	367.0
226.95	671.0
228.95	178.0
243.95	1195.0
244.95	173.0
245.95	214.0
254.95	6749.0
255.95	933.0
257.95	360.0
272.95	266.0
273.95	526.0
274.95	2816.0
275.95	461.0
276.95	269.0
295.95	880.0
322.95	285.0
364.85	328.0
422.95	646.0
440.95	1720.0
441.95	10852.0
442.95	1904.0
443.95	162.0

Instrument :
BNA_G
ClientSampleId :
DFTPP29

m/z	Abundance
40.05	169.0
43.05	151.0
44.05	194.0
49.05	257.0
83.95	322.0
86.05	165.0

Instrument :
BNA_G
ClientSampleId :
DFTPP29