
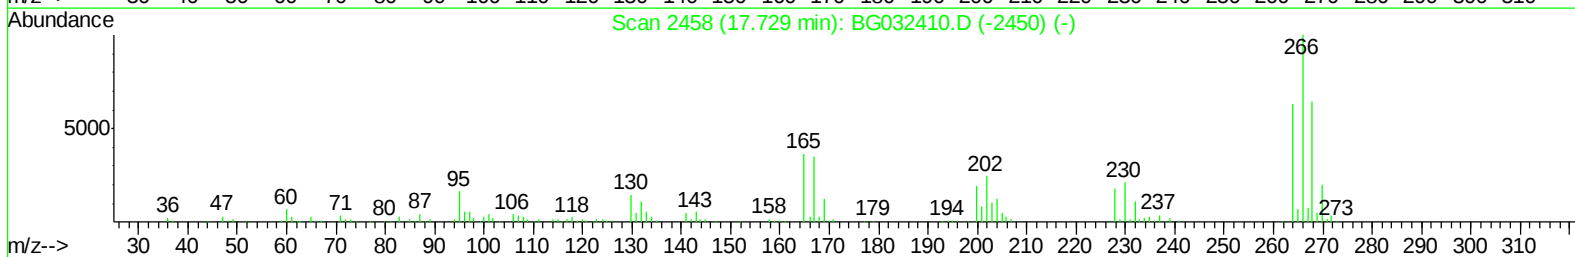
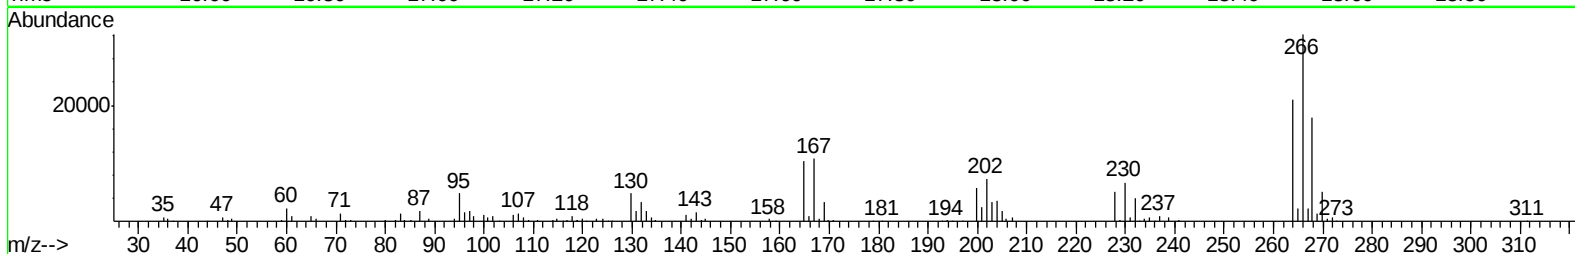


Data Path : Z:\HPCHEM1\BNA G\DATA\BG020818\
Data File : BG032609.D
Acq On : 8 Feb 2018 13:13
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 09 06:47:45 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 18:57:08 2018
Response via : Initial Calibration

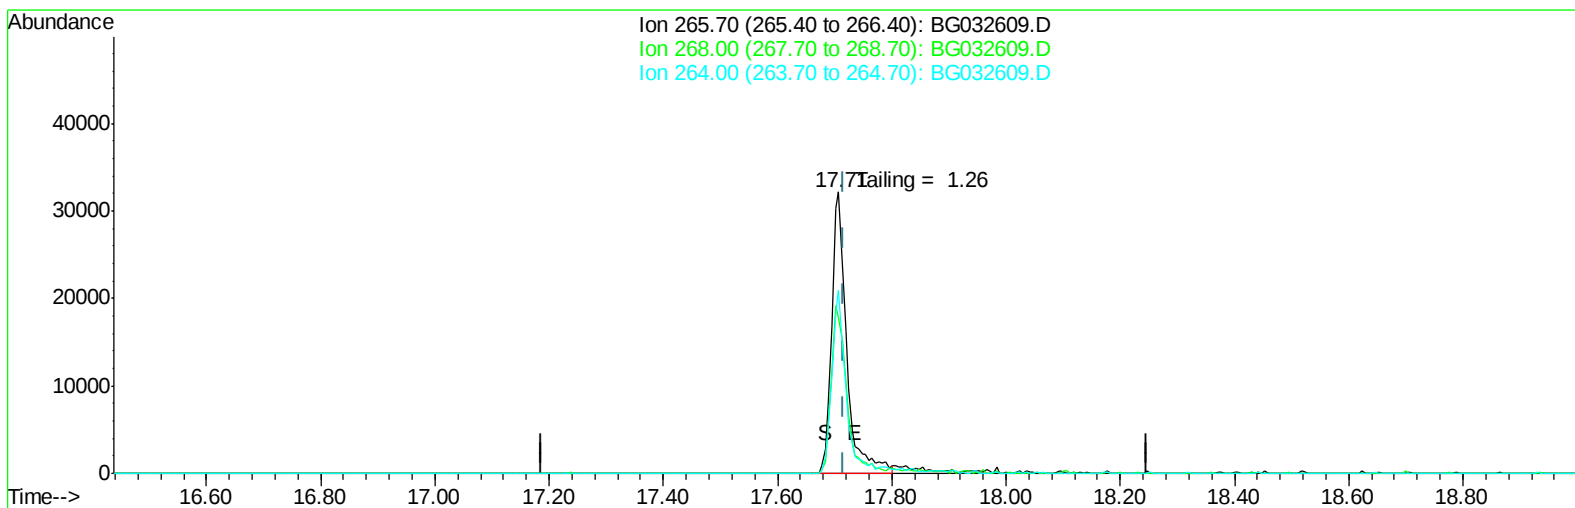

TIC: BG032609.D

(69) Pentachlorophenol (C)




17.707min (-0.010) 95174.61ng

response 58649

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	55.55
264.00	62.00	65.07
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG020818\
Data File : BG032609.D
Acq On : 8 Feb 2018 13:13
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 09 06:47:45 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 18:57:08 2018
Response via : Initial Calibration

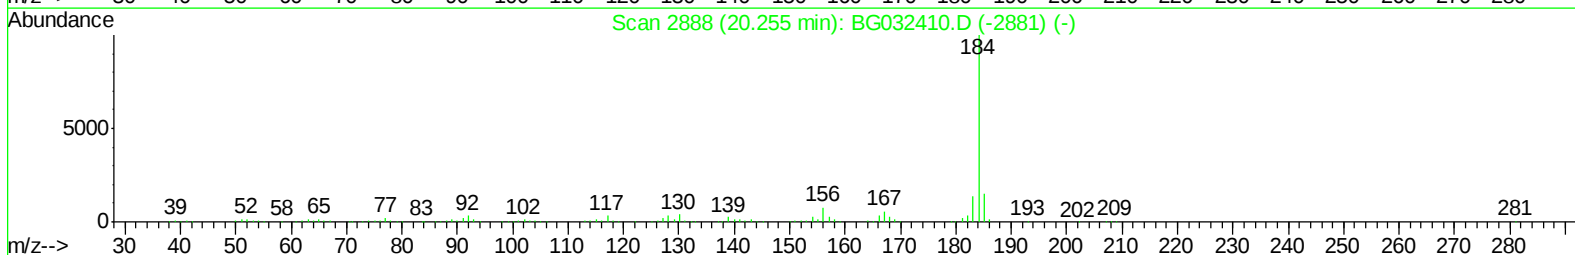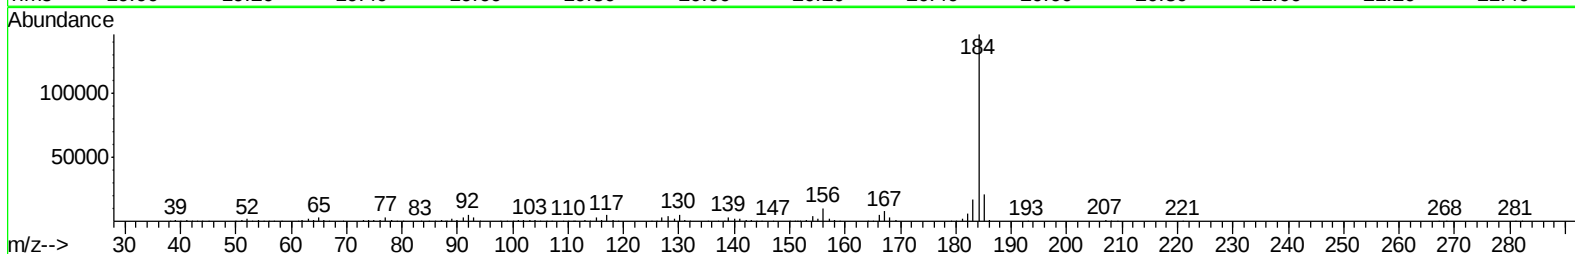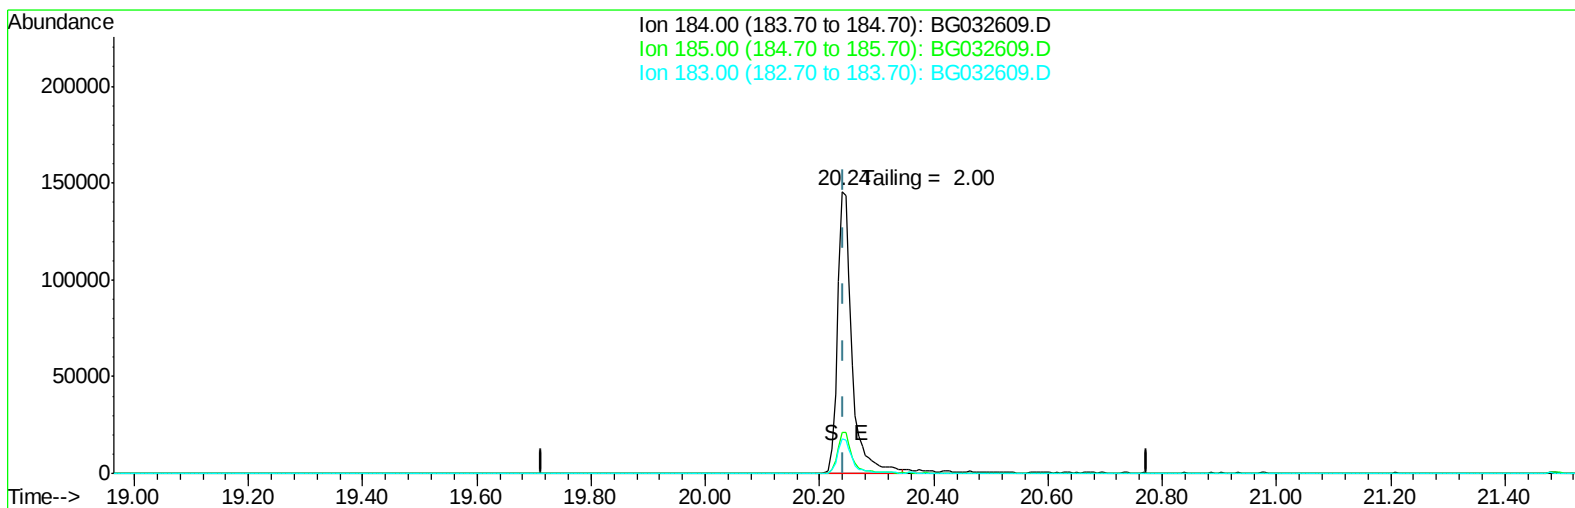

TIC: BG032609.D

(76) Benzidine

20.239min (-0.005) 191227.38ng

response 255336

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.49
183.00	13.30	12.09
0.00	0.00	0.00