
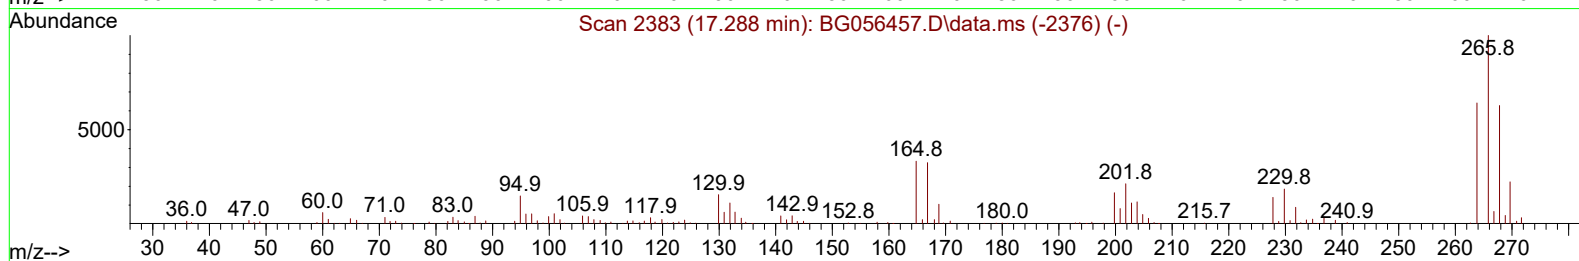
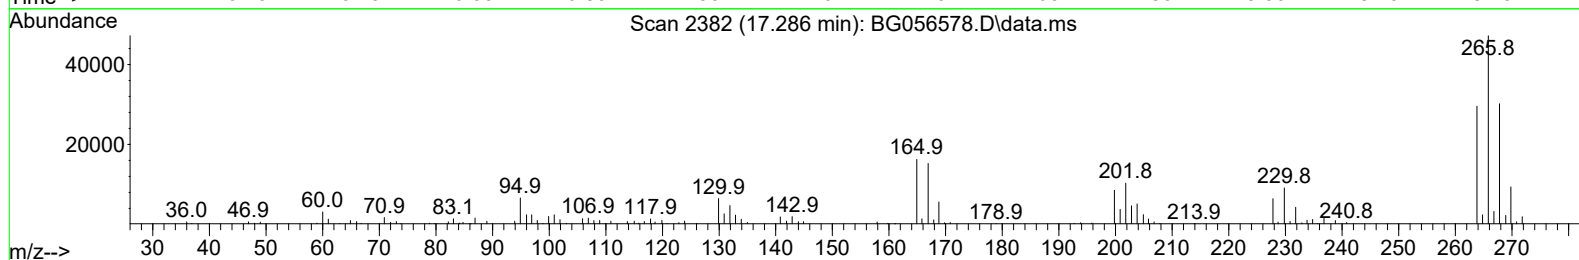


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020823\
Data File : BG056578.D
Acq On : 8 Feb 2023 11:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 09 03:58:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 08 03:02:11 2023
Response via : Initial Calibration

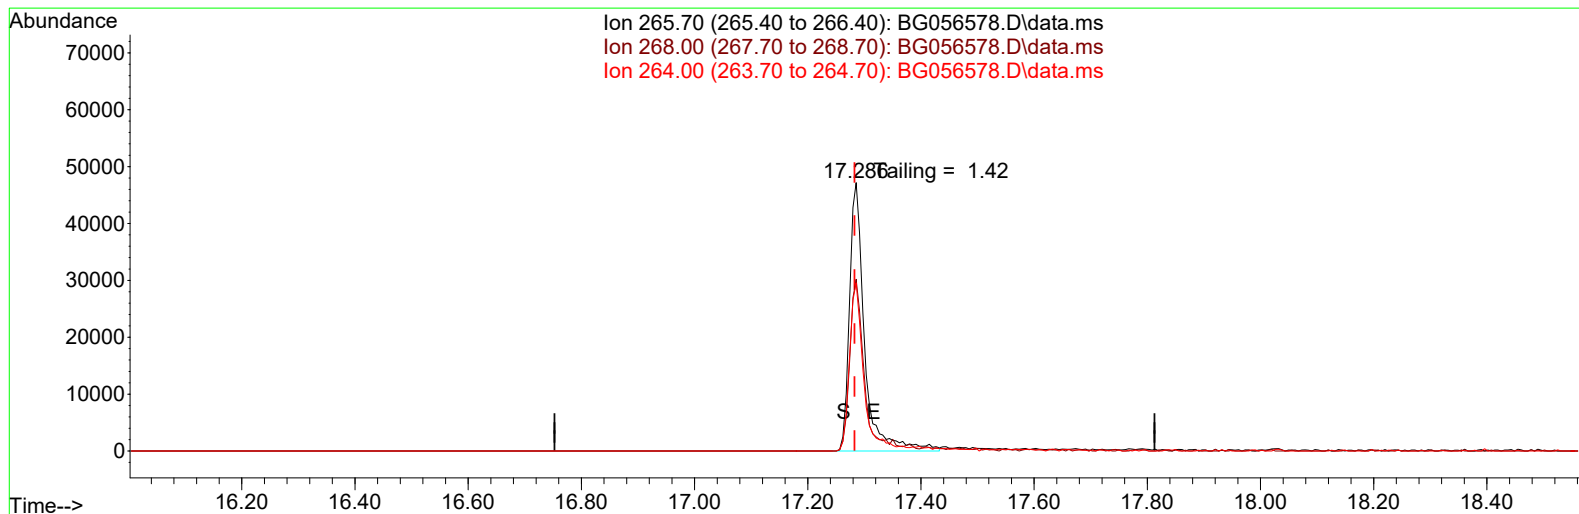

TIC: BG056578.D\data.ms

(70) Pentachlorophenol (C)




17.286min (+ 0.003) 24983.64 ng

response 86622

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	63.97
264.00	64.20	62.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020823\
Data File : BG056578.D
Acq On : 8 Feb 2023 11:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 09 03:58:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 08 03:02:11 2023
Response via : Initial Calibration

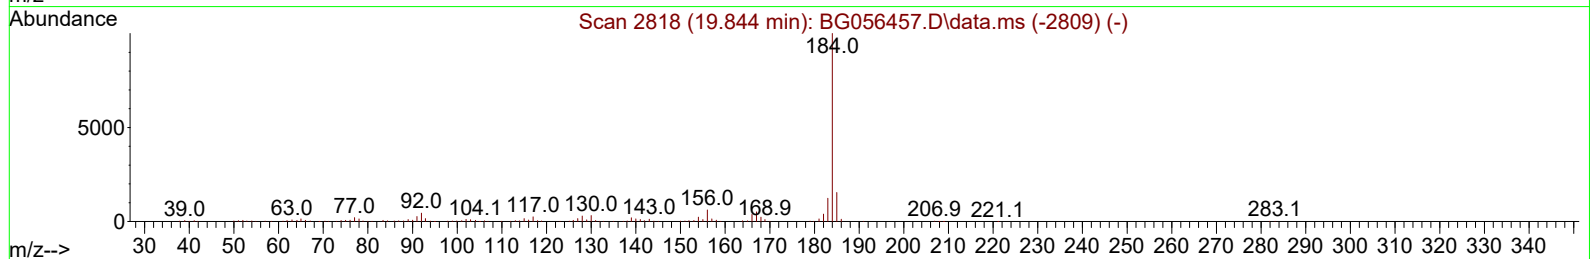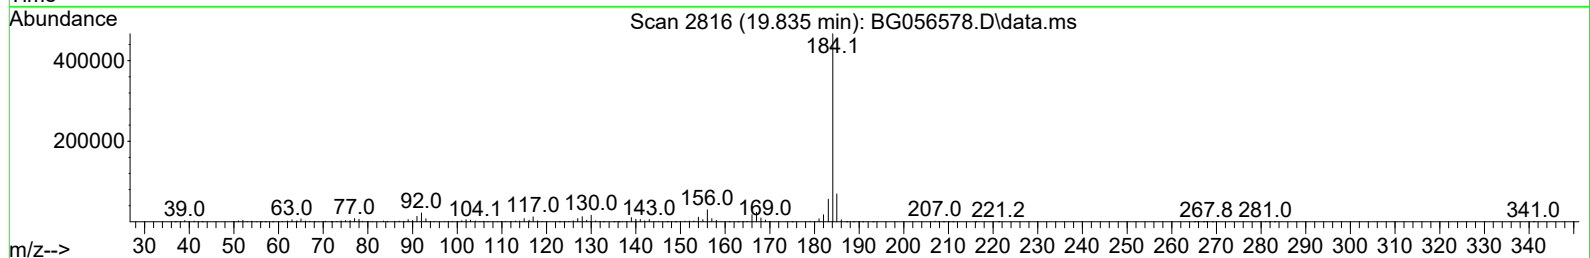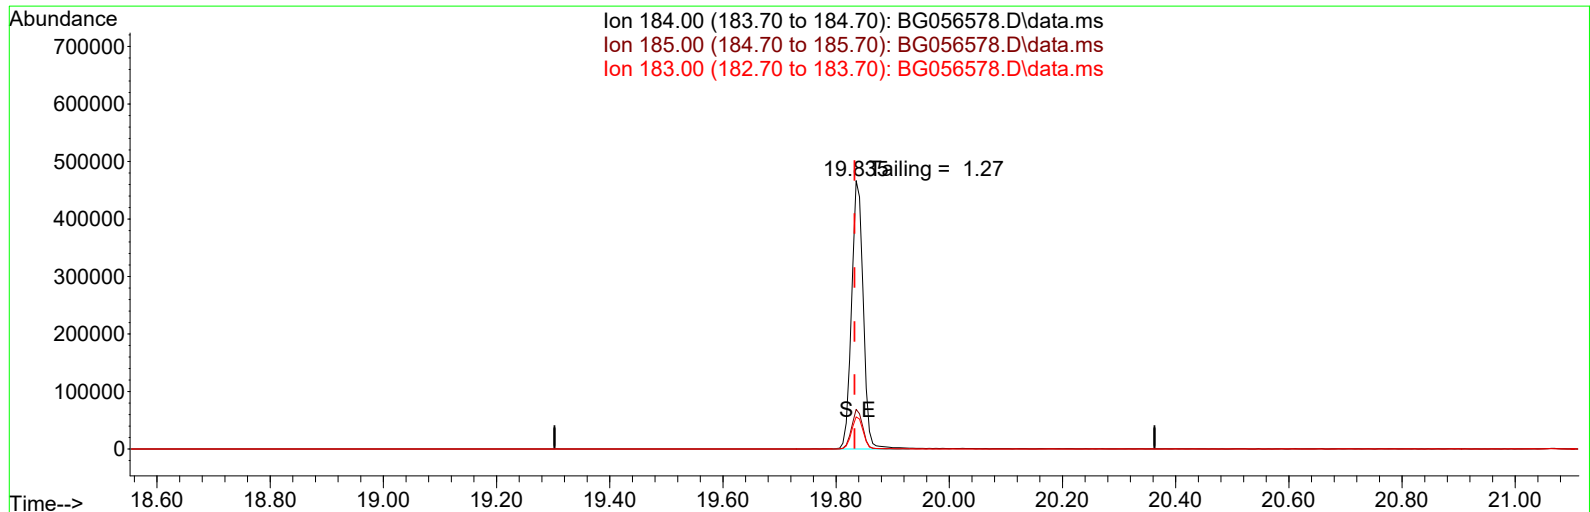

TIC: BG056578.D\data.ms

(77) Benzidine

19.835min (+ 0.003) 381041.59 ng

response 670244

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.82
183.00	12.30	12.01
0.00	0.00	0.00