

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020823\
 Data File : BG056592.D
 Acq On : 8 Feb 2023 22:03
 Operator : CG/JU
 Sample : 01481-07 5X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JPP-42-020723

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG056592.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.303	338	343	349	rBV	21383	32303	4.26%	0.632%
2	5.791	420	426	437	rBV	83265	140791	18.56%	2.756%
3	7.418	696	703	720	rBB	82013	146753	19.34%	2.872%
4	8.270	839	848	856	rBB	133688	228714	30.15%	4.477%
5	9.445	1041	1048	1058	rBV	52163	90730	11.96%	1.776%
6	11.102	1322	1330	1337	rBV	177401	312942	41.25%	6.125%
7	13.511	1733	1740	1749	rBB	202318	294840	38.86%	5.771%
8	14.892	1966	1975	1982	rBV	311286	479433	63.20%	9.384%
9	15.932	2145	2152	2157	rVB2	5493	8461	1.12%	0.166%
10	16.226	2197	2202	2209	rVB	10594	14898	1.96%	0.292%
11	16.373	2220	2227	2234	rBV	112672	175236	23.10%	3.430%
12	17.630	2434	2441	2445	rBV	403289	586756	77.34%	11.485%
13	17.671	2445	2448	2454	rVB	78935	112049	14.77%	2.193%
14	17.765	2459	2464	2468	rVB	18986	26913	3.55%	0.527%
15	18.035	2503	2510	2515	rBV2	8063	18821	2.48%	0.368%
16	18.500	2584	2589	2594	rVV	15253	26900	3.55%	0.527%
17	18.547	2594	2597	2603	rVV2	18758	26617	3.51%	0.521%
18	18.623	2607	2610	2614	rBV2	6993	9706	1.28%	0.190%
19	18.693	2617	2622	2626	rVV3	18448	37289	4.92%	0.730%
20	18.729	2626	2628	2631	rVB2	8864	9845	1.30%	0.193%
21	18.981	2667	2671	2677	rBV	13223	20402	2.69%	0.399%
22	19.034	2677	2680	2684	rBV5	10001	13451	1.77%	0.263%
23	19.404	2736	2743	2746	rBV3	13296	34268	4.52%	0.671%
24	19.669	2782	2788	2793	rVB	187054	262274	34.57%	5.134%
25	19.992	2838	2843	2845	rBV3	32869	57087	7.52%	1.117%
26	20.027	2845	2849	2856	rVB	174813	252744	33.31%	4.947%
27	20.203	2874	2879	2885	rBV	345279	430849	56.79%	8.433%
28	21.919	3163	3171	3176	rBV3	384596	758651	100.00%	14.849%
29	25.350	3748	3755	3764	rVB	178306	499236	65.81%	9.772%




Sum of corrected areas: 5108959

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020823\
Data File : BG056592.D
Acq On : 8 Feb 2023 22:03
Operator : CG/JU
Sample : 01481-07 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JPP-42-020723

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

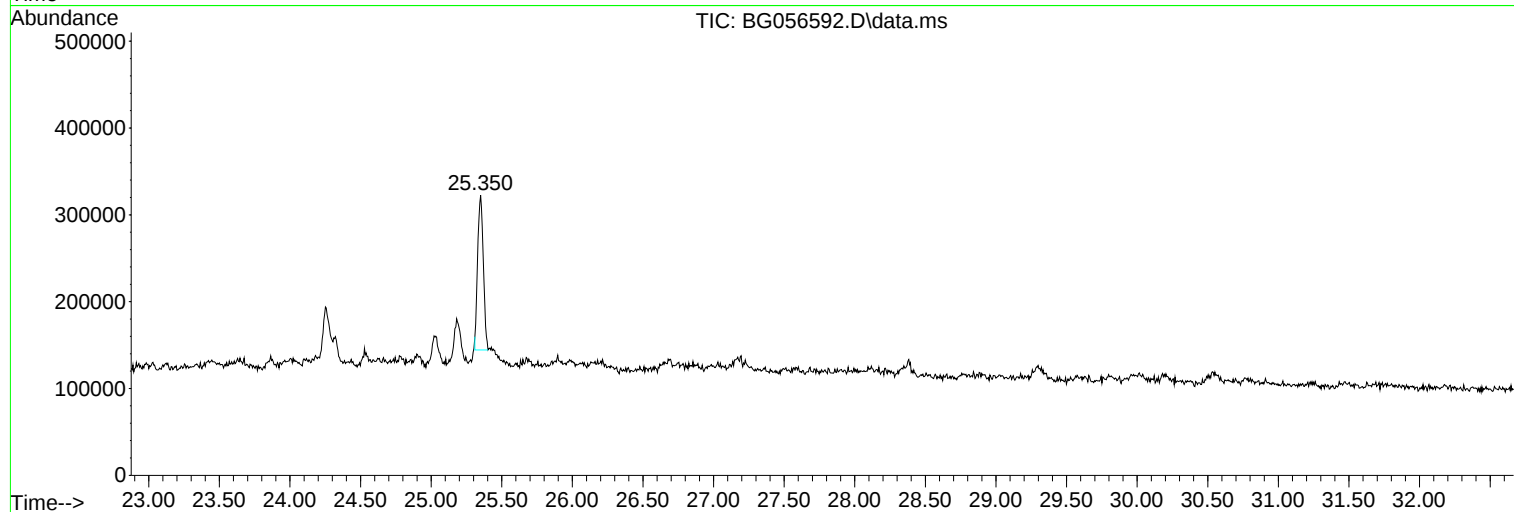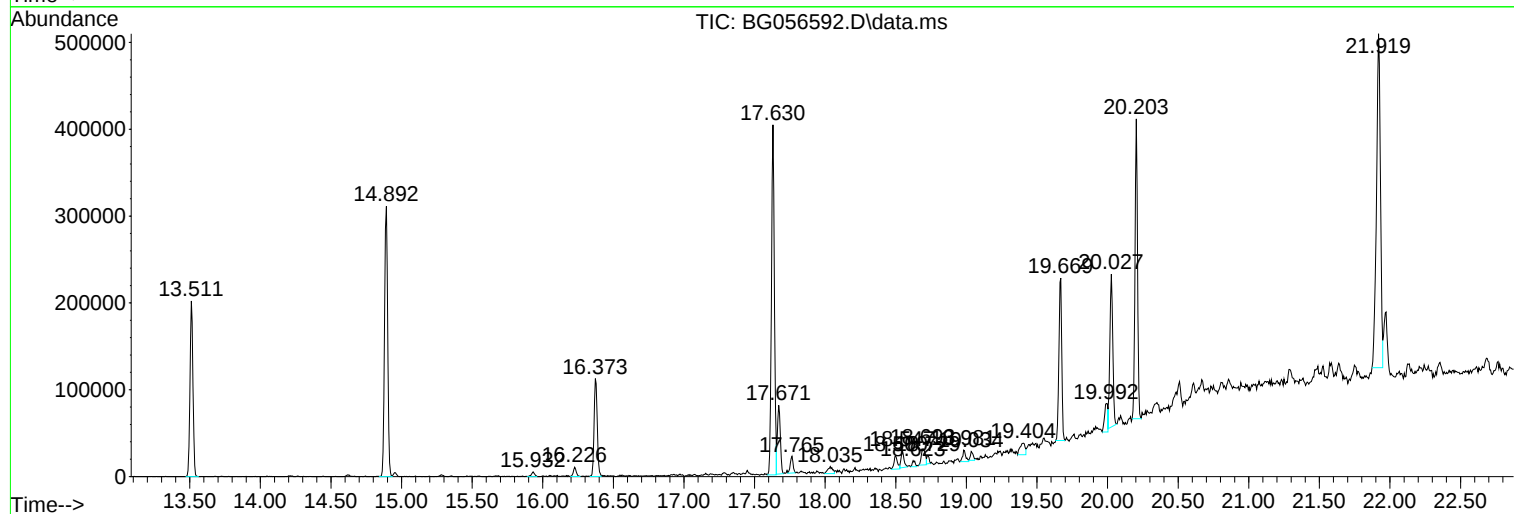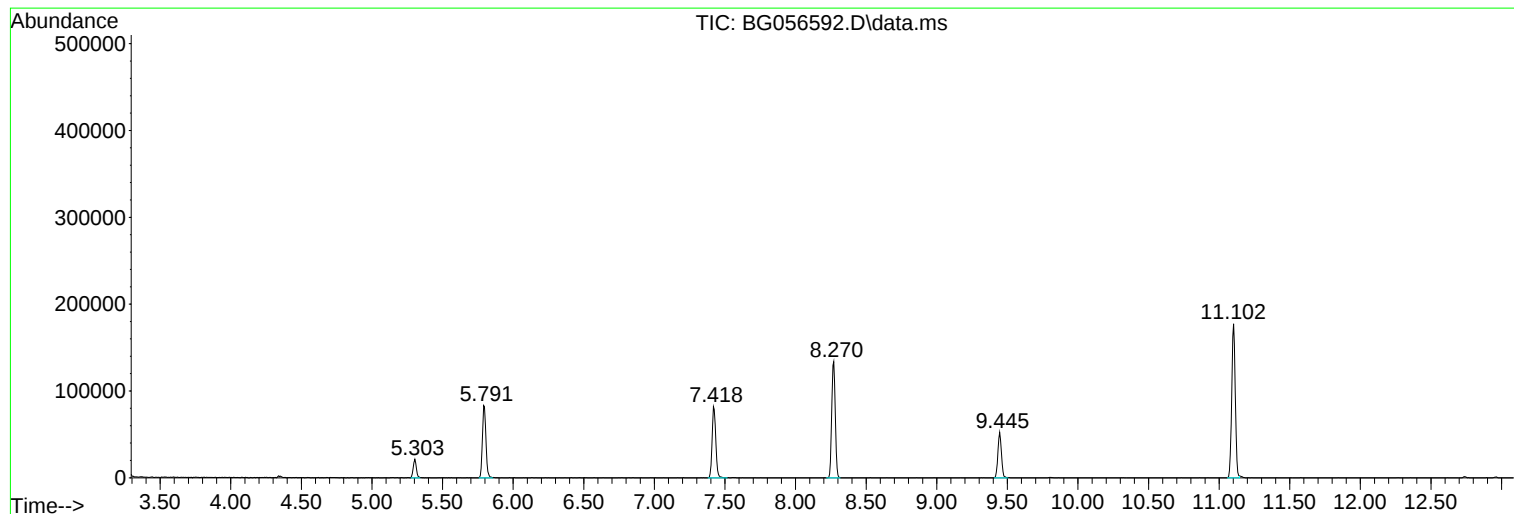

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020823\
Data File : BG056592.D
Acq On : 8 Feb 2023 22:03
Operator : CG/JU
Sample : 01481-07 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JPP-42-020723










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.303	2.82 ng	32303	1,4-Dichlorobenzene-d4	8.270

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	47		
2	Isopropyldimethylsilane	102	C5H14Si	1000433-69-3	38		
3	Butanoic acid, 4-(2-methoxy-1-me...	204	C9H16O5	054966-46-0	36		
4	1,2-Butanediol	90	C4H10O2	000584-03-2	17		
5	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	17		

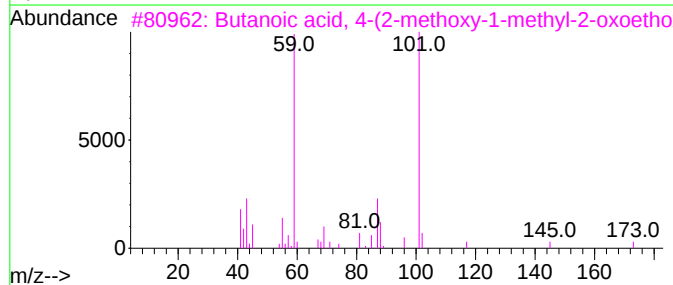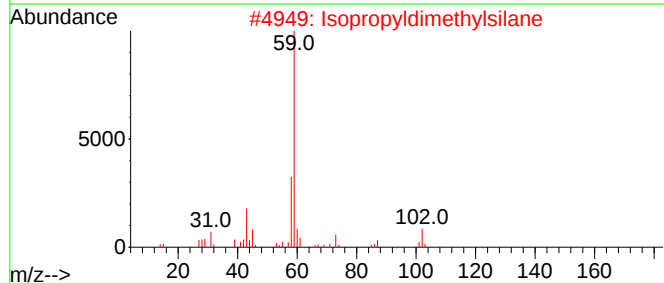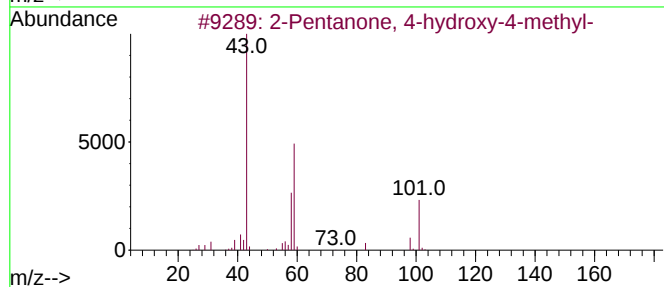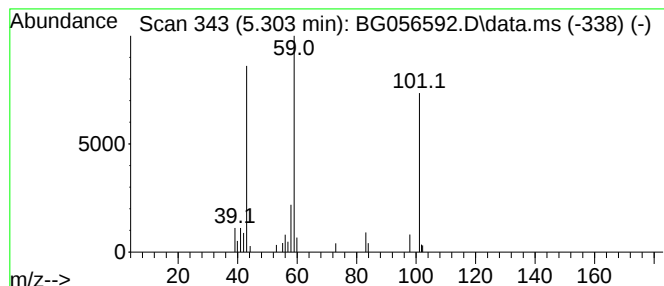

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020823\
Data File : BG056592.D
Acq On : 8 Feb 2023 22:03
Operator : CG/JU
Sample : 01481-07 5X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JPP-42-020723

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.303	2.8	ng	32303	1	8.270	228714	20.0