


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020823\
Data File : BG056578.D
Acq On : 8 Feb 2023 11:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Feb 08 03:02:11 2023

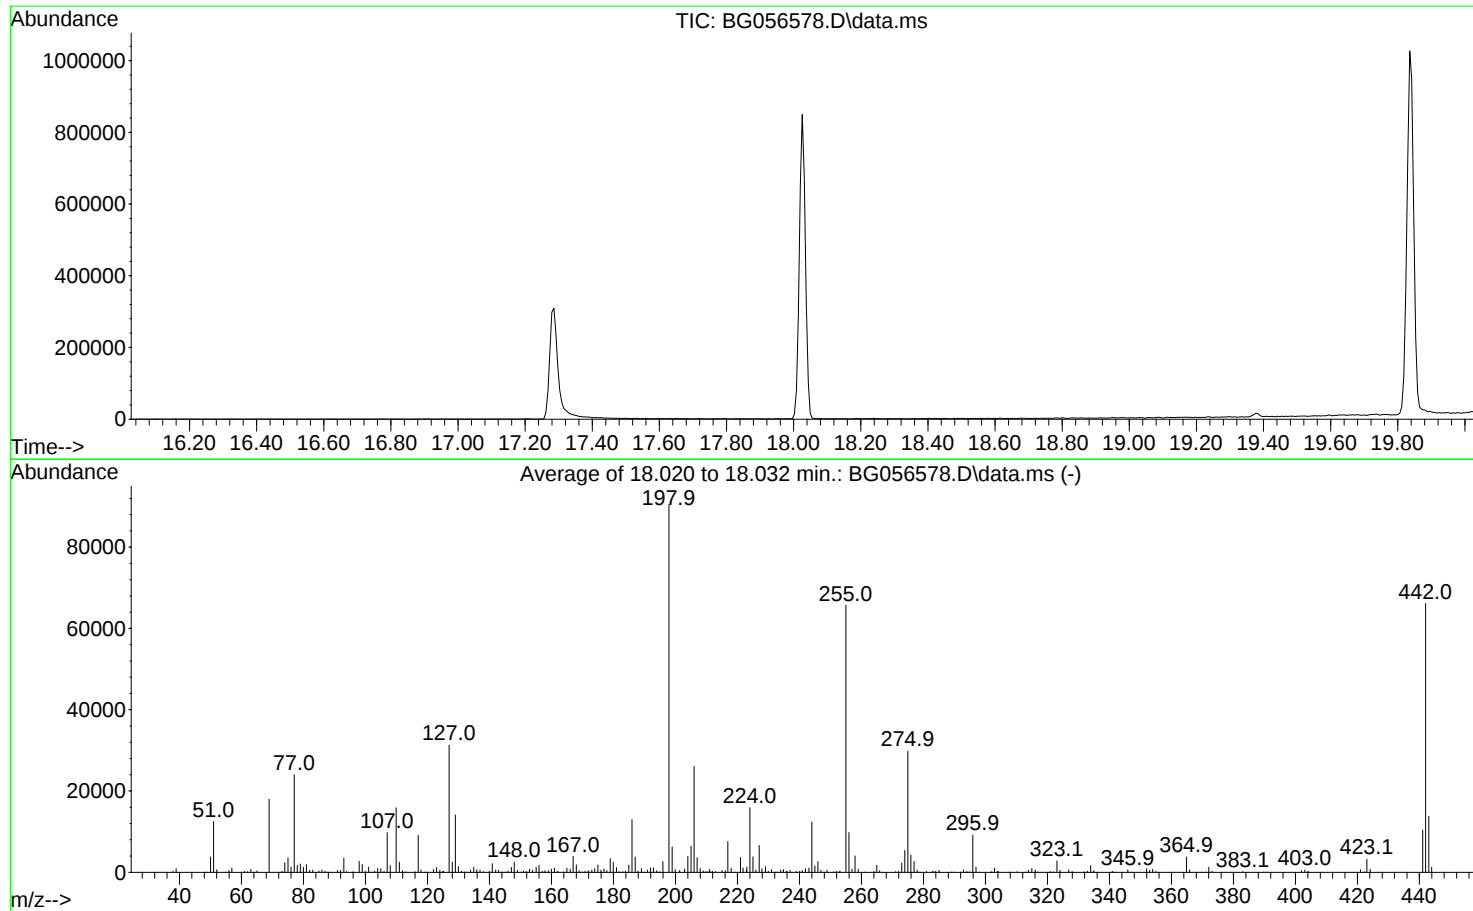




AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2500

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	13.8	12487	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	19.9	17977	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	34.6	31283	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	90507	PASS
199	198	5	9	6.9	6246	PASS
275	198	10	60	32.9	29797	PASS
365	198	1	100	4.1	3755	PASS
441	198	0.01	100	11.5	10412	PASS
442	442	50	100	100.0	66104	PASS
443	442	15	24	20.8	13778	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020823\
Data File : BG056578.D
Acq On : 8 Feb 2023 11:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 09 03:58:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 08 03:02:11 2023
Response via : Initial Calibration

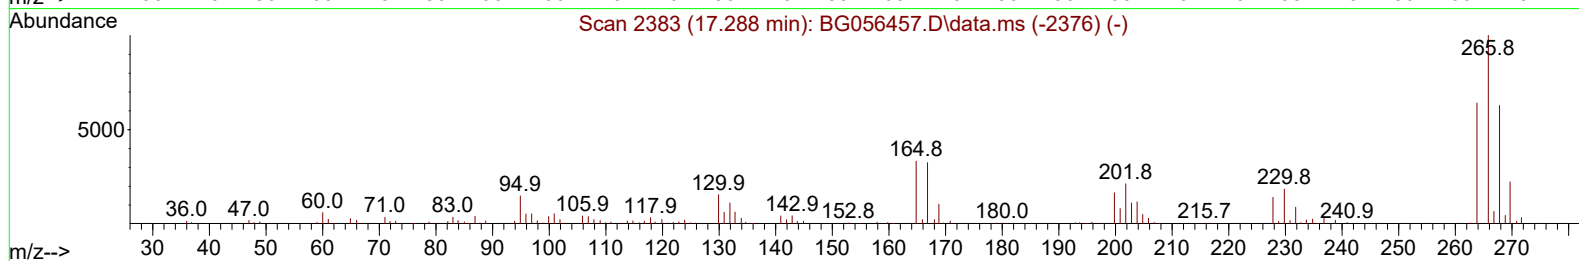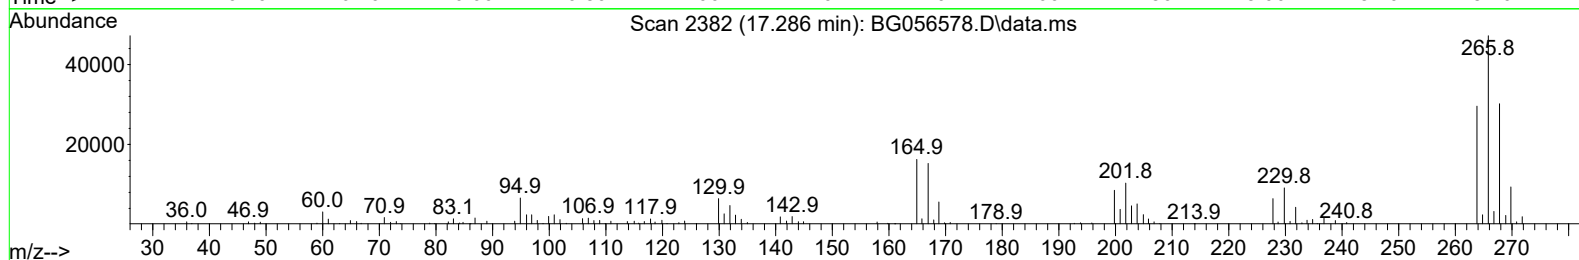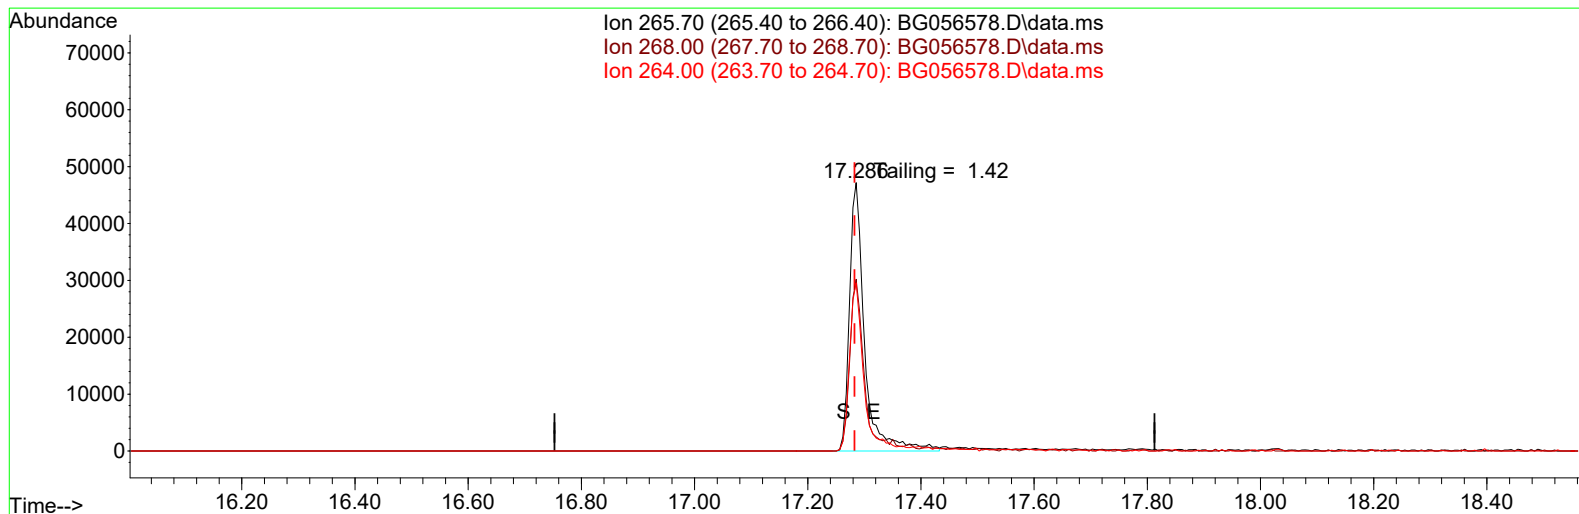

TIC: BG056578.D\data.ms

(70) Pentachlorophenol (C)

17.286min (+ 0.003) 24983.64 ng




response 86622

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	63.97
264.00	64.20	62.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020823\
Data File : BG056578.D
Acq On : 8 Feb 2023 11:29
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 09 03:58:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG012723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 08 03:02:11 2023
Response via : Initial Calibration

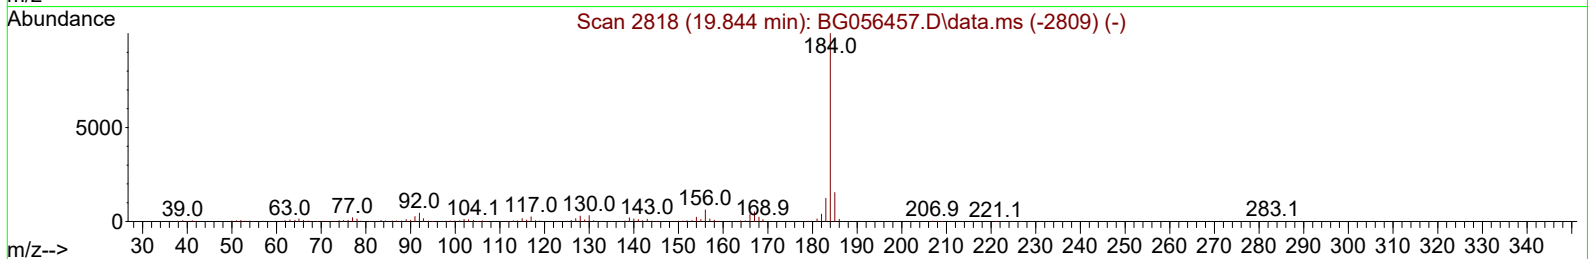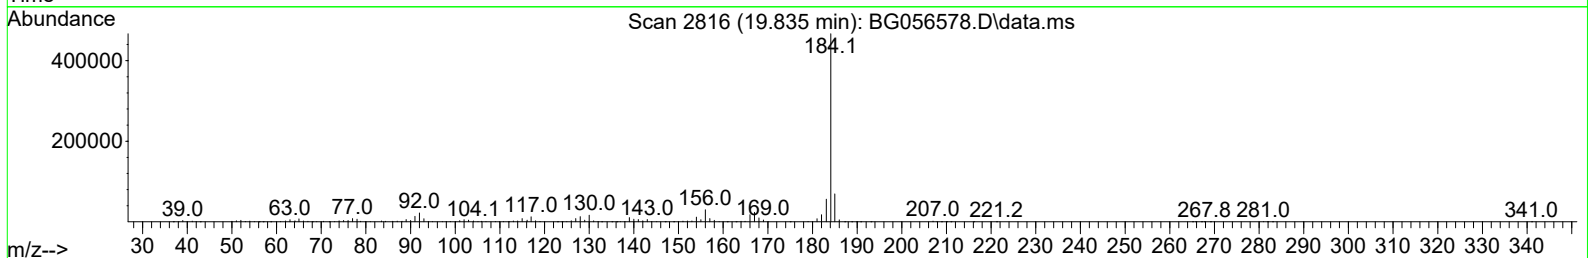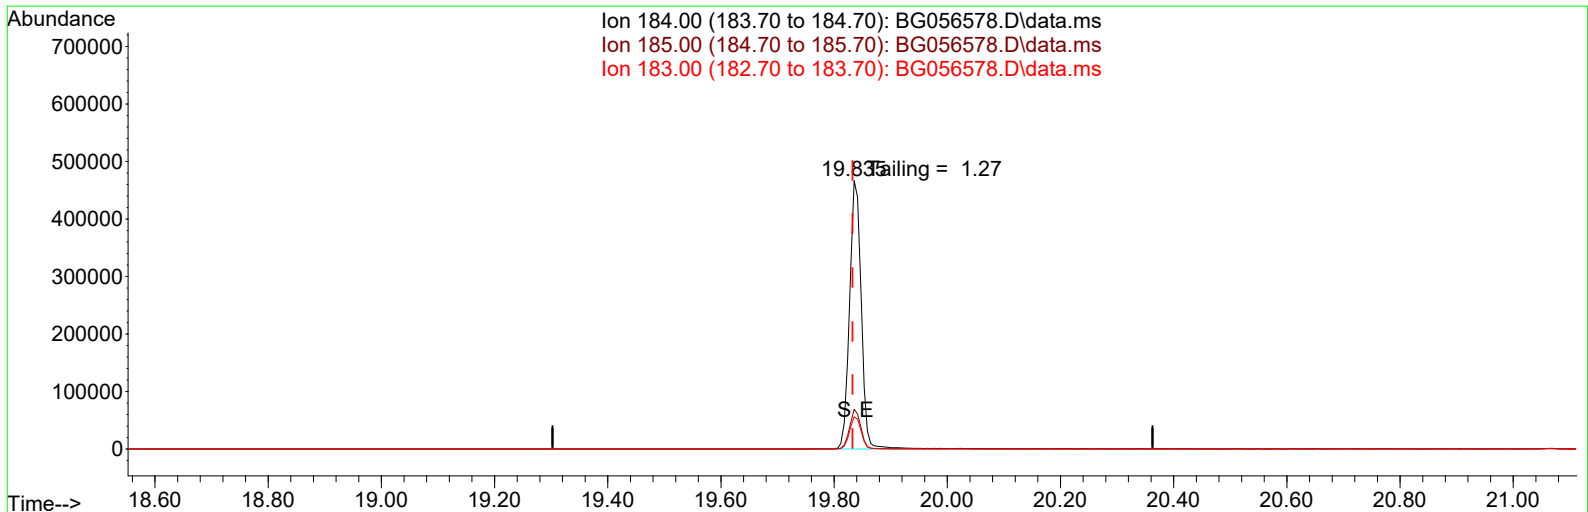

TIC: BG056578.D\data.ms

(77) Benzidine

19.835min (+ 0.003) 381041.59 ng

response 670244

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.40	14.82
183.00	12.30	12.01
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/8/2023	BNA_G	<u>BG056578.D</u>
Compound Name	Response	Retention Time
DDT	306122	21.063
DDD	9644	20.617
DDE	1059	20.112
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10703	316825	3.38

Instrument :
BNA_G
ClientSampleId :
DFTPP