

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG020916\
 Data File : BG020818.D
 Acq On : 9 Feb 2016 15:29
 Operator : SJ/UM
 Sample : H1371-22
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C04L8

Quant Time: Feb 10 00:17:55 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG020816.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 10 00:13:30 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.27	152	17053	20.00	ng/ul	0.00
18) Naphthalene-d8	11.10	136	86702	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.89	164	54596	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.62	188	123160	20.00	ng/ul	0.00
78) Chrysene-d12	21.90	240	115993	20.00	ng/ul	0.00
86) Perylene-d12	25.28	264	107379	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.61	96	2003	5.70	ng/uL	0.00
5) Phenol-d5	7.40	99	50253	29.09	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.58	67	29126	31.60	ng/ul	0.00
9) 2-Chlorophenol-d4	7.80	132	40613	30.04	ng/ul	0.00
13) 4-Methylphenol-d8	8.96	113	44787	29.82	ng/ul	0.00
19) Nitrobenzene-d5	9.44	128	22265	32.00	ng/ul	0.00
22) 2-Nitrophenol-d4	10.16	143	19981	28.88	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.70	165	39051	29.32	ng/ul	0.00
29) 4-Chloroaniline-d4	11.22	131	33739	19.03	ng/ul	0.00
44) Dimethylphthalate-d6	14.28	166	142338	30.30	ng/ul	0.00
47) Acenaphthylene-d8	14.58	160	192198	33.49	ng/ul	0.00
52) 4-Nitrophenol-d4	15.05	143	28082	29.86	ng/ul	0.00
58) Fluorene-d10	15.87	176	136889	34.24	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.97	200	12946	21.69	ng/ul	0.00
71) Anthracene-d10	17.72	188	210828	34.65	ng/ul	0.00
79) Pyrene-d10	19.99	212	213293	35.77	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.06	264	210054	35.30	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.33	163	67614	13.82	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG020916\
Data File : BG020818.D
Acq On : 9 Feb 2016 15:29
Operator : SJ/UM
Sample : H1371-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C04L8

Quant Time: Feb 10 00:17:55 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG020816.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 10 00:13:30 2016
Response via : Initial Calibration

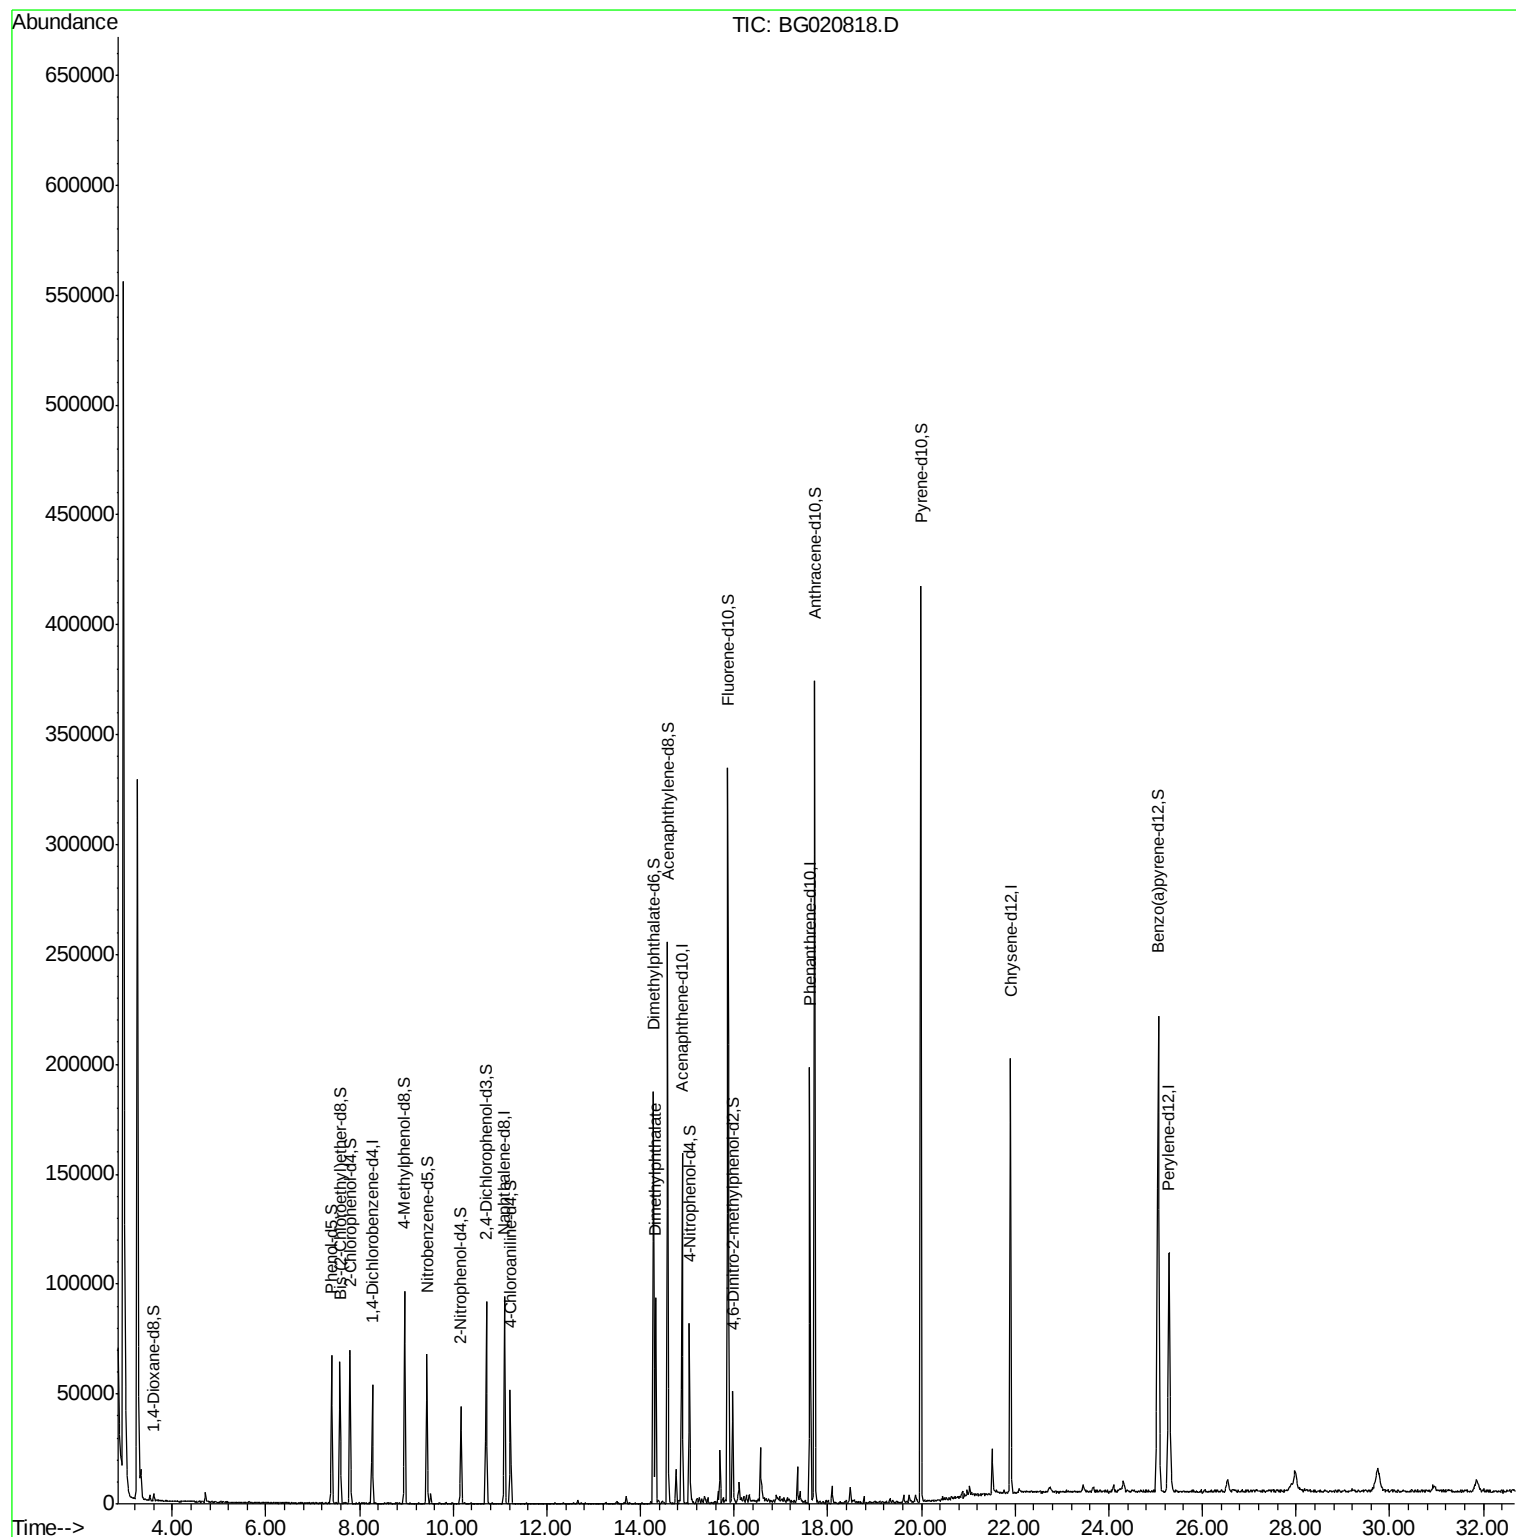

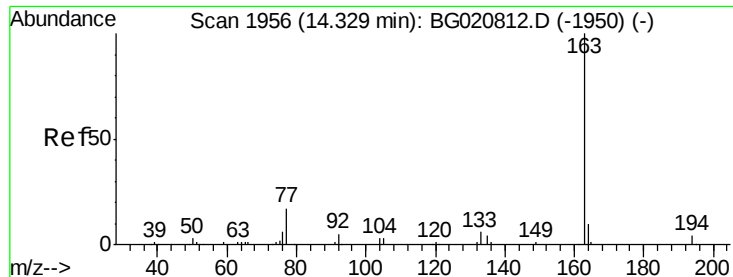

#45

Dimethylphthalate

Concen: 13.82 ng/ul

RT: 14.33 min Scan# 1956

Delta R.T. -0.00 min

Lab File: BG020818.D

Acq: 9 Feb 2016 15:29

Instrument :

BNA_G

ClientSampleId :

C04L8


Tgt Ion:163 Resp: 67614

Ion Ratio Lower Upper

163 100

194 3.8 3.0 4.6

164 10.1 7.7 11.5

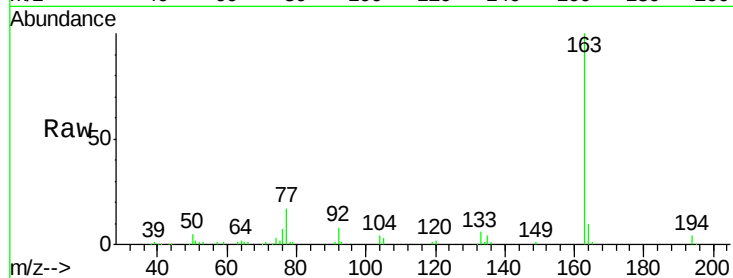

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

