

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG020916\
 Data File : BG020829.D
 Acq On : 9 Feb 2016 22:40
 Operator : SJ/UM
 Sample : H1371-12
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C04H7

Quant Time: Feb 10 00:41:19 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG020816.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 10 00:34:52 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.27	152	21973	20.00	ng/ul	0.00
18) Naphthalene-d8	11.10	136	114483	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.89	164	66842	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.62	188	130819	20.00	ng/ul	0.00
78) Chrysene-d12	21.91	240	111354	20.00	ng/ul	0.00
86) Perylene-d12	25.30	264	105779	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.60	96	2160	4.77	ng/uL	0.00
5) Phenol-d5	7.41	99	57234	25.72	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.58	67	31217	26.28	ng/ul	0.00
9) 2-Chlorophenol-d4	7.80	132	47348	27.18	ng/ul	0.00
13) 4-Methylphenol-d8	8.97	113	51874	26.81	ng/ul	0.00
19) Nitrobenzene-d5	9.44	128	25147	27.37	ng/ul	0.00
22) 2-Nitrophenol-d4	10.17	143	27458	30.05	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.71	165	47115	26.79	ng/ul	0.00
29) 4-Chloroaniline-d4	11.23	131	74010	31.61	ng/ul	0.00
44) Dimethylphthalate-d6	14.28	166	160613	27.92	ng/ul	0.00
47) Acenaphthylene-d8	14.58	160	207626	29.55	ng/ul	0.00
52) 4-Nitrophenol-d4	15.05	143	25924	22.51	ng/ul	0.00
58) Fluorene-d10	15.87	176	140921	28.79	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.97	200	12370	19.51	ng/ul	0.00
71) Anthracene-d10	17.72	188	192036	29.71	ng/ul	0.00
79) Pyrene-d10	19.99	212	182192	31.82	ng/ul	0.01
90) Benzo(a)pyrene-d12	25.07	264	176183	30.06	ng/ul	0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.33	163	61614	10.29	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG020916\
Data File : BG020829.D
Acq On : 9 Feb 2016 22:40
Operator : SJ/UM
Sample : H1371-12
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C04H7

Quant Time: Feb 10 00:41:19 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG020816.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 10 00:34:52 2016
Response via : Initial Calibration

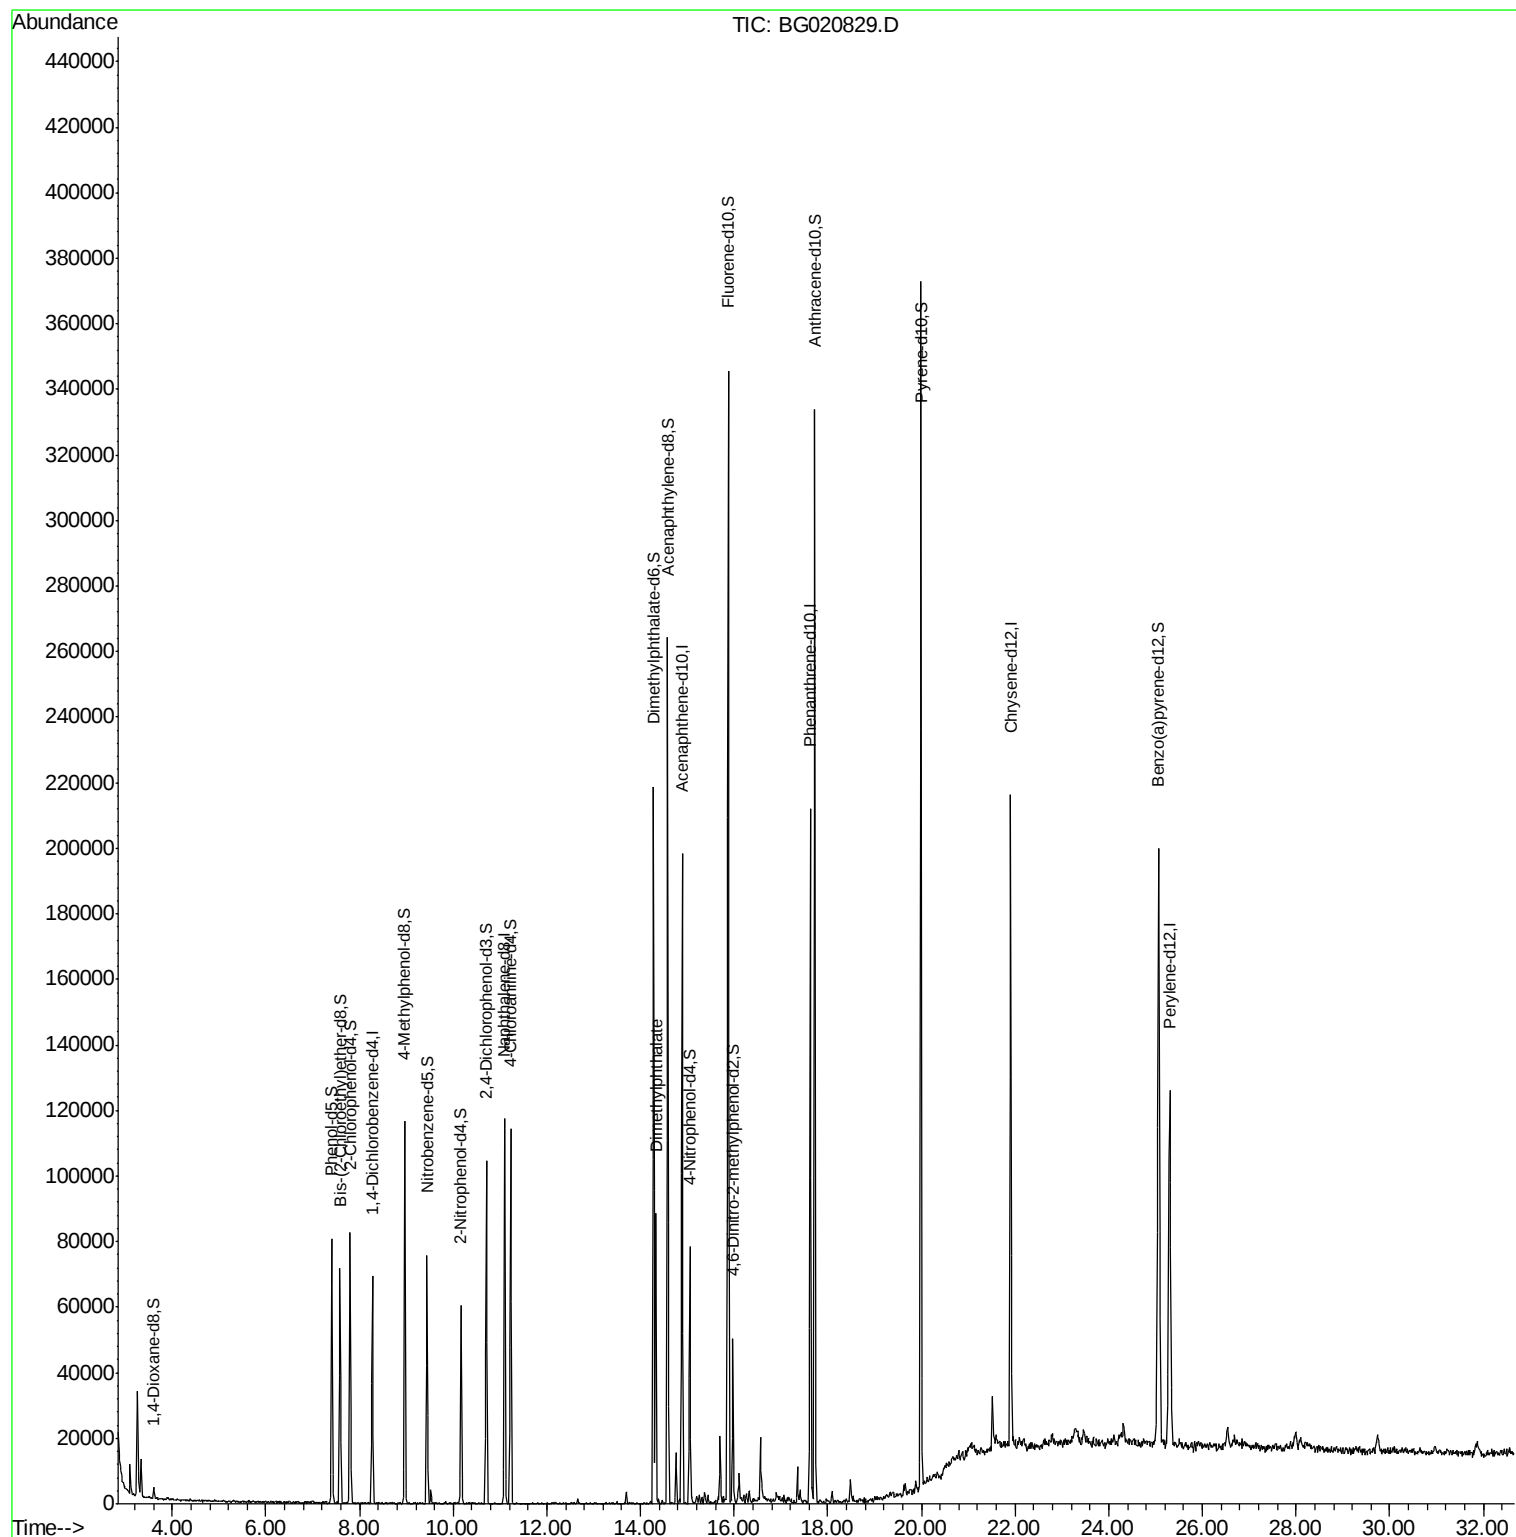

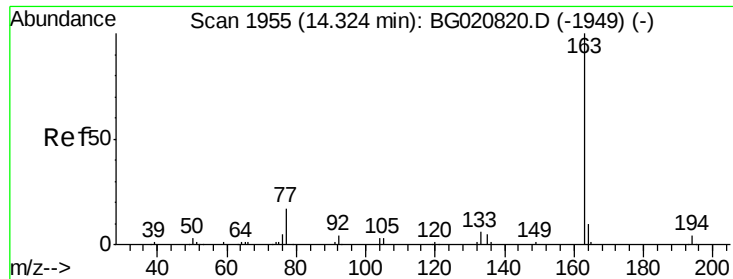

#45

Dimethylphthalate

Concen: 10.29 ng/ul

RT: 14.33 min Scan# 1956

Delta R.T. 0.00 min

Lab File: BG020829.D

Acq: 9 Feb 2016 22:40

Instrument :

BNA_G

ClientSampleId :

C04H7

Tgt Ion:163 Resp: 61614

Ion Ratio Lower Upper

163 100

194 3.9 3.0 4.6

164 10.1 7.7 11.5

