

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG020916\
 Data File : BG020830.D
 Acq On : 9 Feb 2016 23:19
 Operator : SJ/UM
 Sample : H1371-03
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C04L2

Quant Time: Feb 10 00:41:26 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG020816.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 10 00:34:52 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.27	152	20933	20.00	ng/ul	0.00
18) Naphthalene-d8	11.10	136	110049	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.89	164	64441	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.62	188	125359	20.00	ng/ul	0.00
78) Chrysene-d12	21.90	240	109097	20.00	ng/ul	0.00
86) Perylene-d12	25.29	264	104657	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.60	96	2380	5.52	ng/uL	0.00
5) Phenol-d5	7.41	99	65490	30.89	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.59	67	35279	31.18	ng/ul	0.00
9) 2-Chlorophenol-d4	7.80	132	53520	32.25	ng/ul	0.00
13) 4-Methylphenol-d8	8.97	113	58908	31.96	ng/ul	0.00
19) Nitrobenzene-d5	9.44	128	29425	33.32	ng/ul	0.00
22) 2-Nitrophenol-d4	10.17	143	30560	34.79	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.71	165	54703	32.36	ng/ul	0.00
29) 4-Chloroaniline-d4	11.22	131	85826	38.13	ng/ul	0.00
44) Dimethylphthalate-d6	14.28	166	183055	33.01	ng/ul	0.00
47) Acenaphthylene-d8	14.58	160	238548	35.22	ng/ul	0.00
52) 4-Nitrophenol-d4	15.05	143	32858	29.60	ng/ul	0.00
58) Fluorene-d10	15.88	176	159841	33.88	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.98	200	15489	25.50	ng/ul	0.00
71) Anthracene-d10	17.72	188	220440	35.59	ng/ul	0.00
79) Pyrene-d10	19.99	212	212583	37.90	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.07	264	205614	35.45	ng/ul	0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.33	163	75692	13.11	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG020916\
Data File : BG020830.D
Acq On : 9 Feb 2016 23:19
Operator : SJ/UM
Sample : H1371-03
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C04L2

Quant Time: Feb 10 00:41:26 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG020816.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 10 00:34:52 2016
Response via : Initial Calibration

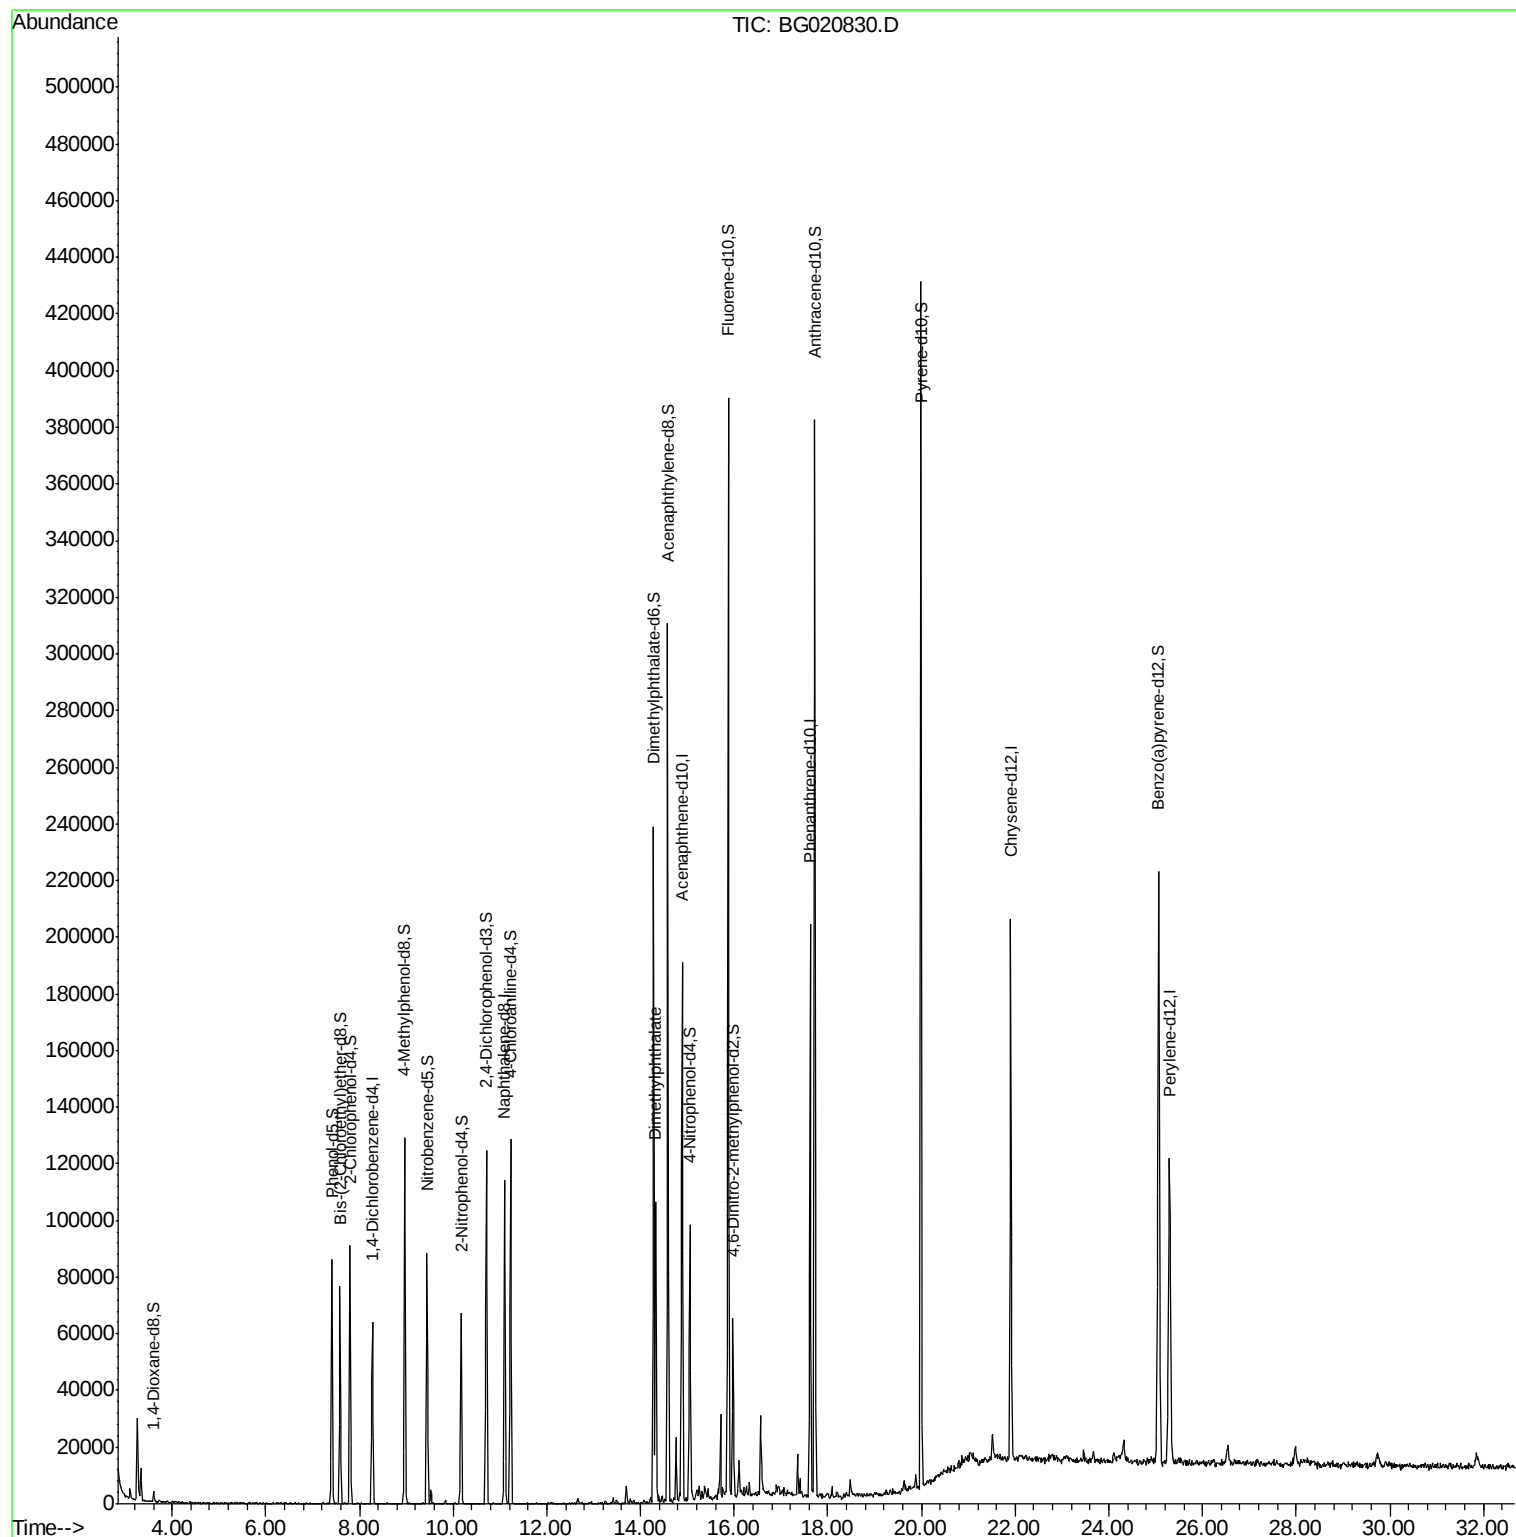

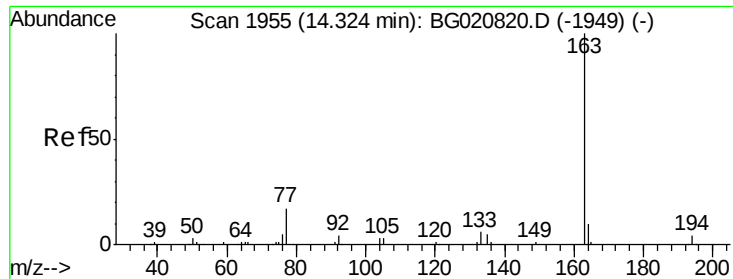

#45

Dimethylphthalate

Concen: 13.11 ng/ul

RT: 14.33 min Scan# 1956

Delta R.T. 0.01 min

Lab File: BG020830.D

Acq: 9 Feb 2016 23:19

Instrument :

BNA_G

ClientSampleId :

C04L2


Tgt Ion:163 Resp: 75692

Ion Ratio Lower Upper

163 100

194 3.9 3.0 4.6

164 9.7 7.7 11.5

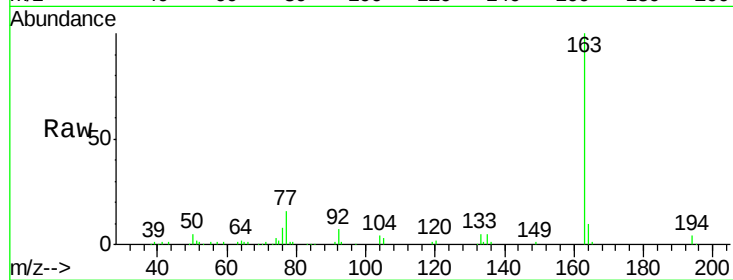

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

