

Data Path : Z:\HPCHEM1\BNA G\DATA\BG020916\
 Data File : BG020814.D
 Acq On : 9 Feb 2016 12:52
 Operator : SJ/UM
 Sample : H1371-04
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C04L3

Quant Time: Feb 10 00:17:28 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG020816.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 10 00:13:30 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.27	152	17476	20.00	ng/ul	0.00
18) Naphthalene-d8	11.10	136	86533	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.89	164	53079	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.62	188	119358	20.00	ng/ul	0.00
78) Chrysene-d12	21.90	240	109846	20.00	ng/ul	0.00
86) Perylene-d12	25.29	264	102324	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.61	96	1821	5.06	ng/uL	0.00
5) Phenol-d5	7.40	99	50519	28.54	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.58	67	24442	25.87	ng/ul	0.00
9) 2-Chlorophenol-d4	7.80	132	40408	29.17	ng/ul	0.00
13) 4-Methylphenol-d8	8.97	113	37598	24.43	ng/ul	0.00
19) Nitrobenzene-d5	9.44	128	21748	31.32	ng/ul	0.00
22) 2-Nitrophenol-d4	10.17	143	19275	27.91	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.70	165	33023	24.84	ng/ul	0.00
29) 4-Chloroaniline-d4	11.22	131	53784	30.39	ng/ul	0.00
44) Dimethylphthalate-d6	14.28	166	127443	27.90	ng/ul	0.00
47) Acenaphthylene-d8	14.58	160	152920	27.41	ng/ul	0.00
52) 4-Nitrophenol-d4	15.05	143	22221	24.30	ng/ul	0.00
58) Fluorene-d10	15.87	176	106653	27.44	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.97	200	11168	19.31	ng/ul	0.00
71) Anthracene-d10	17.72	188	162618	27.57	ng/ul	0.00
79) Pyrene-d10	19.99	212	158962	28.15	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.06	264	154957	27.33	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.33	163	48864	10.27	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG020916\
Data File : BG020814.D
Acq On : 9 Feb 2016 12:52
Operator : SJ/UM
Sample : H1371-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C04L3

Quant Time: Feb 10 00:17:28 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG020816.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 10 00:13:30 2016
Response via : Initial Calibration

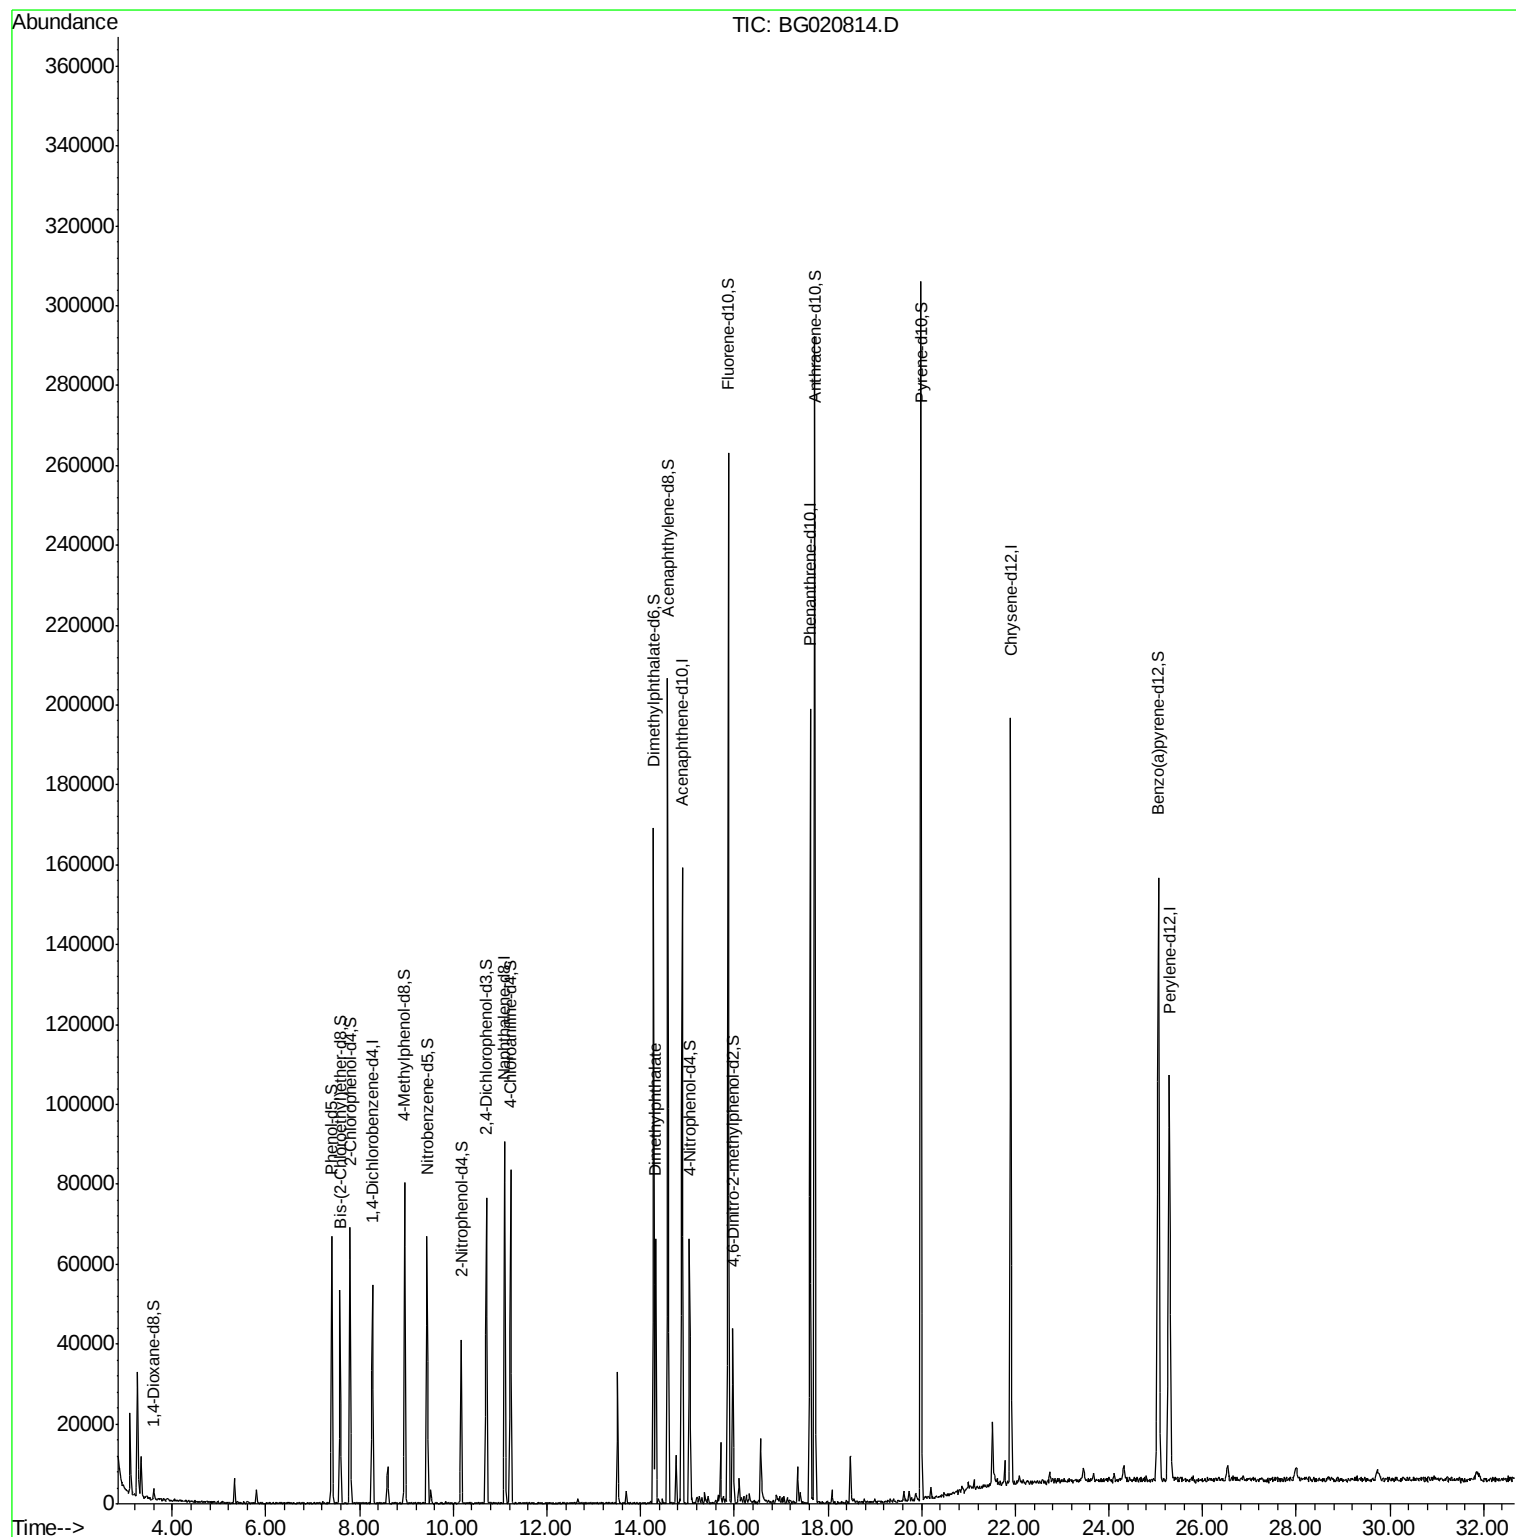


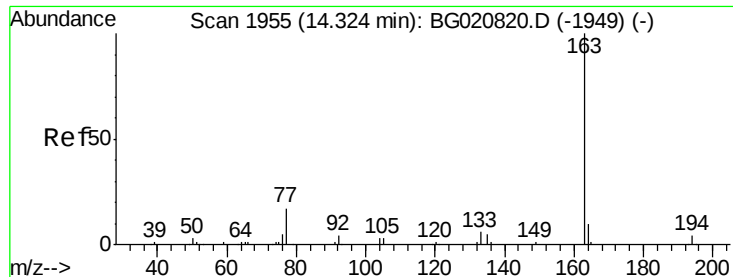

#45
 Dimethylphthalate
 Concen: 10.27 ng/ul
 RT: 14.33 min Scan# 1956
 Delta R.T. -0.00 min
 Lab File: BG020814.D
 Acq: 9 Feb 2016 12:52

Instrument :
 BNA_G
 ClientSampleId :
 C04L3

Tot Ion:163 Resp: 48864
 Ion Ratio Lower Upper
 163 100
 194 3.7 3.0 4.6
 164 9.7 7.7 11.5

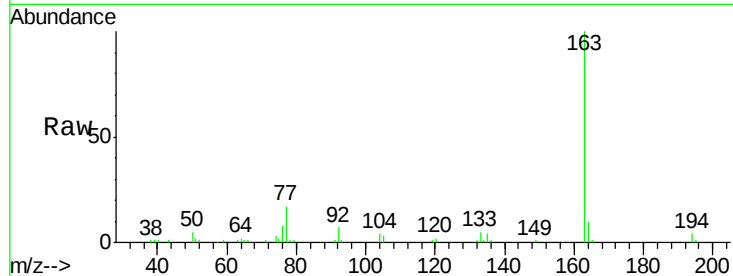

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

