

Data Path : Z:\HPCHEM1\BNA G\DATA\BG020916\
 Data File : BG020815.D
 Acq On : 9 Feb 2016 13:32
 Operator : SJ/UM
 Sample : H1371-13
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C04H8

Quant Time: Feb 10 00:17:34 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG020816.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 10 00:13:30 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.27	152	16859	20.00	ng/ul	0.00
18) Naphthalene-d8	11.10	136	85469	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.89	164	52864	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.62	188	118469	20.00	ng/ul	0.00
78) Chrysene-d12	21.91	240	107613	20.00	ng/ul	0.00
86) Perylene-d12	25.29	264	100368	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.61	96	2090	6.02	ng/uL	0.00
5) Phenol-d5	7.41	99	44557	26.09	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.58	67	27045	29.68	ng/ul	0.00
9) 2-Chlorophenol-d4	7.79	132	37696	28.21	ng/ul	0.00
13) 4-Methylphenol-d8	8.96	113	40705	27.42	ng/ul	0.00
19) Nitrobenzene-d5	9.44	128	20598	30.03	ng/ul	0.00
22) 2-Nitrophenol-d4	10.17	143	21108	30.94	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.70	165	36544	27.84	ng/ul	0.00
29) 4-Chloroaniline-d4	11.22	131	61526	35.19	ng/ul	0.00
44) Dimethylphthalate-d6	14.28	166	143666	31.58	ng/ul	0.00
47) Acenaphthylene-d8	14.58	160	172068	30.97	ng/ul	0.00
52) 4-Nitrophenol-d4	15.05	143	24702	27.12	ng/ul	0.00
58) Fluorene-d10	15.87	176	121703	31.44	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.97	200	13261	23.10	ng/ul	0.00
71) Anthracene-d10	17.72	188	184414	31.50	ng/ul	0.00
79) Pyrene-d10	19.98	212	181254	32.76	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.05	264	178294	32.06	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.33	163	44443	9.38	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG020916\
Data File : BG020815.D
Acq On : 9 Feb 2016 13:32
Operator : SJ/UM
Sample : H1371-13
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C04H8

Quant Time: Feb 10 00:17:34 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG020816.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 10 00:13:30 2016
Response via : Initial Calibration

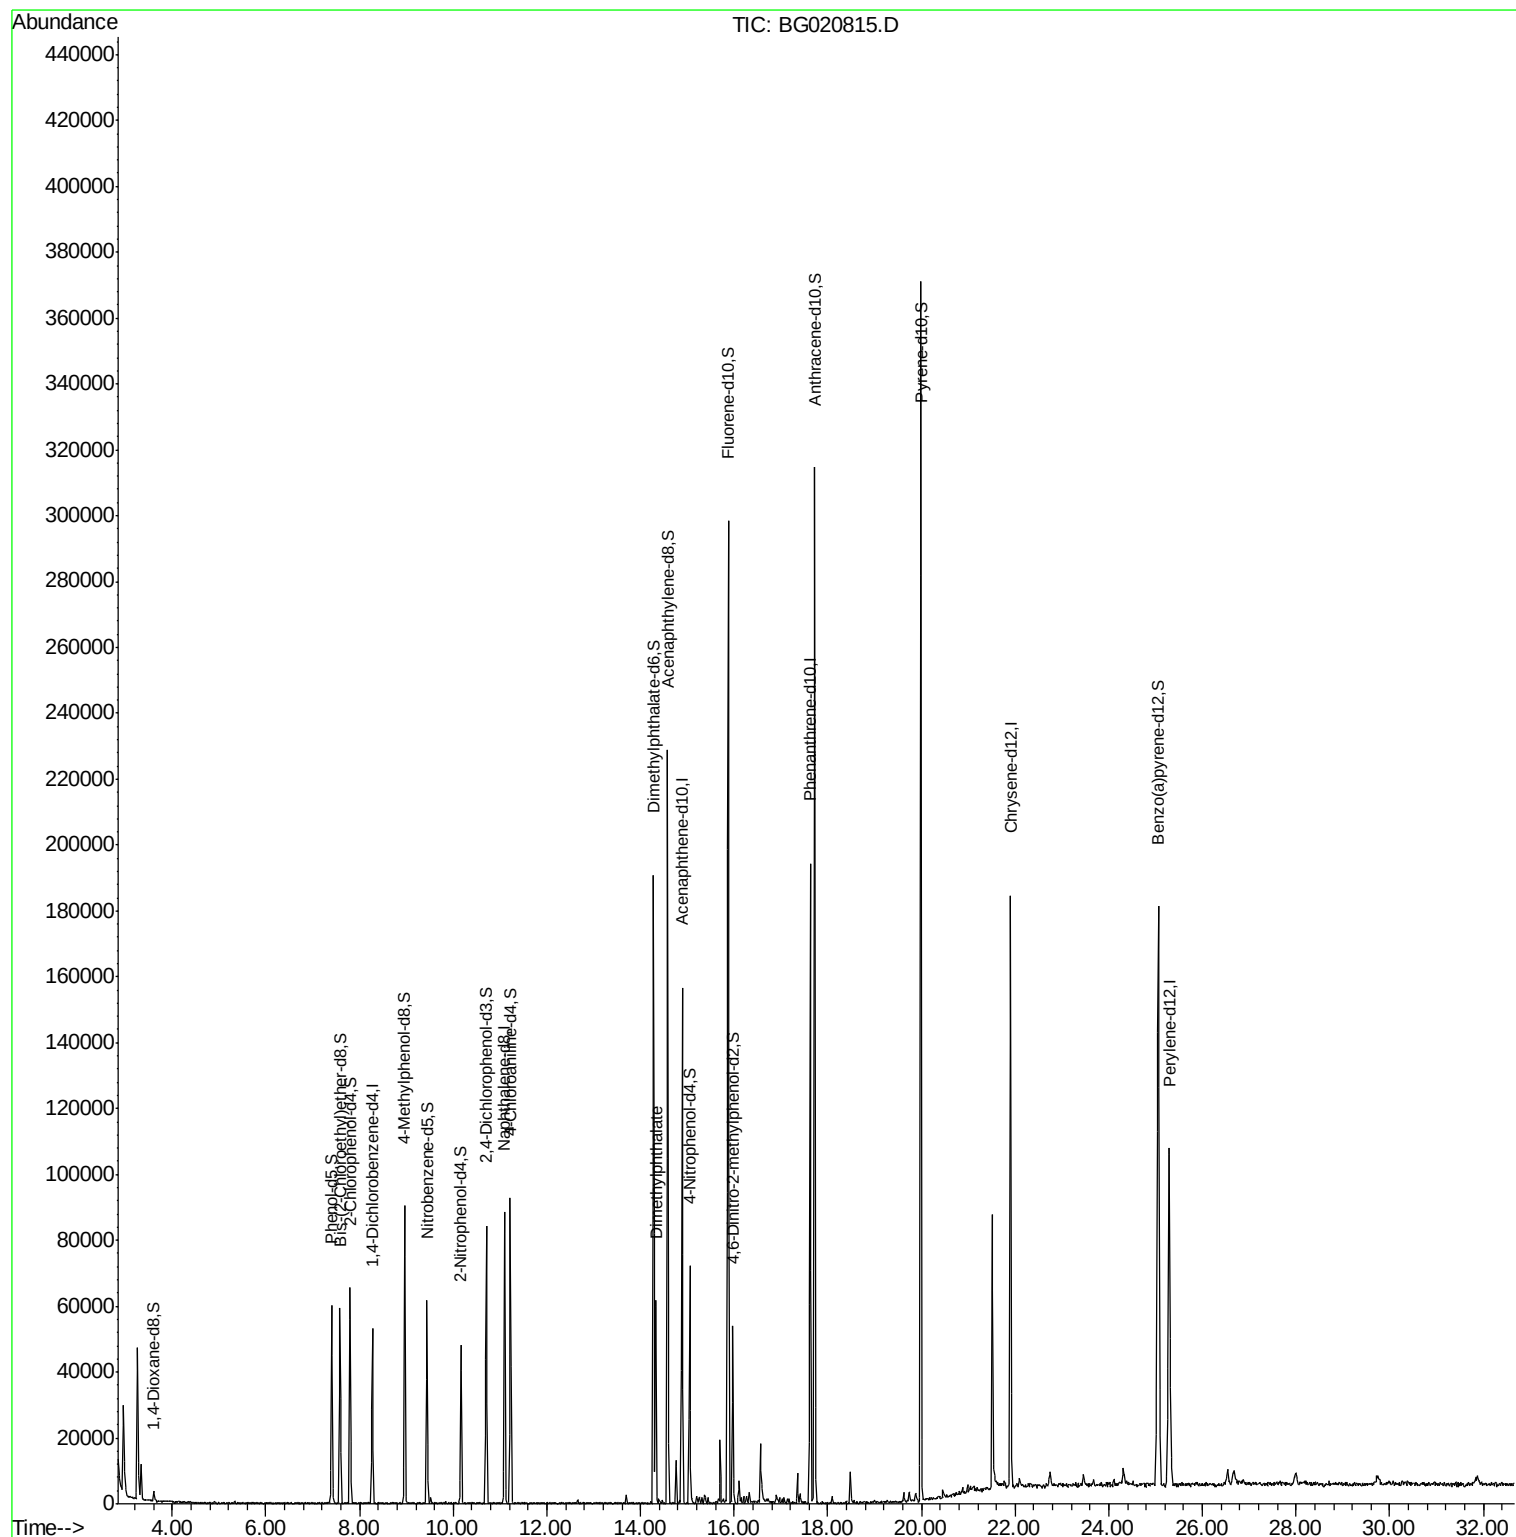

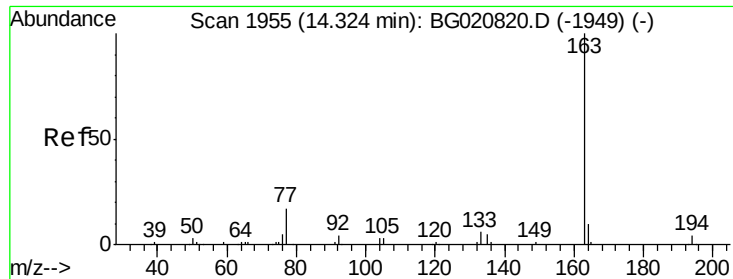

#45

Dimethylphthalate

Concen: 9.38 ng/ul

RT: 14.33 min Scan# 1956

Delta R.T. -0.00 min

Lab File: BG020815.D

Acq: 9 Feb 2016 13:32

Instrument :

BNA_G

ClientSampleId :

C04H8


Tot Ion:163 Resp: 44443

Ion Ratio Lower Upper

163 100

194 3.8 3.0 4.6

164 9.5 7.7 11.5

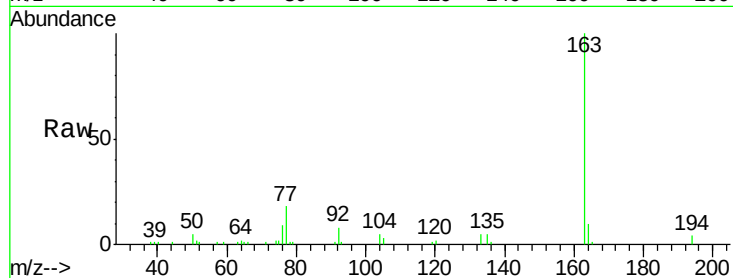

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

