

Data Path : Z:\HPCHEM1\BNA G\DATA\BG020916\
 Data File : BG020816.D
 Acq On : 9 Feb 2016 14:11
 Operator : SJ/UM
 Sample : H1371-14
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C04H9

Quant Time: Feb 10 00:17:41 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG020816.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 10 00:13:30 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.27	152	15439	20.00	ng/ul	0.00
18) Naphthalene-d8	11.10	136	76835	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.88	164	48769	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.62	188	113863	20.00	ng/ul	0.00
78) Chrysene-d12	21.90	240	105115	20.00	ng/ul	0.00
86) Perylene-d12	25.29	264	98880	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.60	96	1828	5.75	ng/uL	0.00
5) Phenol-d5	7.40	99	42242	27.01	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.58	67	25805	30.92	ng/ul	0.00
9) 2-Chlorophenol-d4	7.80	132	35322	28.86	ng/ul	0.00
13) 4-Methylphenol-d8	8.96	113	38158	28.07	ng/ul	0.00
19) Nitrobenzene-d5	9.44	128	19295	31.29	ng/ul	0.00
22) 2-Nitrophenol-d4	10.17	143	20661	33.69	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.70	165	34560	29.28	ng/ul	0.00
29) 4-Chloroaniline-d4	11.22	131	59708	37.99	ng/ul	0.00
44) Dimethylphthalate-d6	14.28	166	144527	34.44	ng/ul	0.00
47) Acenaphthylene-d8	14.58	160	168391	32.85	ng/ul	0.00
52) 4-Nitrophenol-d4	15.05	143	26361	31.38	ng/ul	0.00
58) Fluorene-d10	15.87	176	121169	33.93	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.97	200	14041	25.45	ng/ul	0.00
71) Anthracene-d10	17.72	188	190356	33.84	ng/ul	0.00
79) Pyrene-d10	19.99	212	191624	35.46	ng/ul	0.00
90) Benzo(a)pyrene-d12	25.06	264	188129	34.33	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	14.32	163	56534	12.94	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG020916\
Data File : BG020816.D
Acq On : 9 Feb 2016 14:11
Operator : SJ/UM
Sample : H1371-14
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C04H9

Quant Time: Feb 10 00:17:41 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG020816.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 10 00:13:30 2016
Response via : Initial Calibration

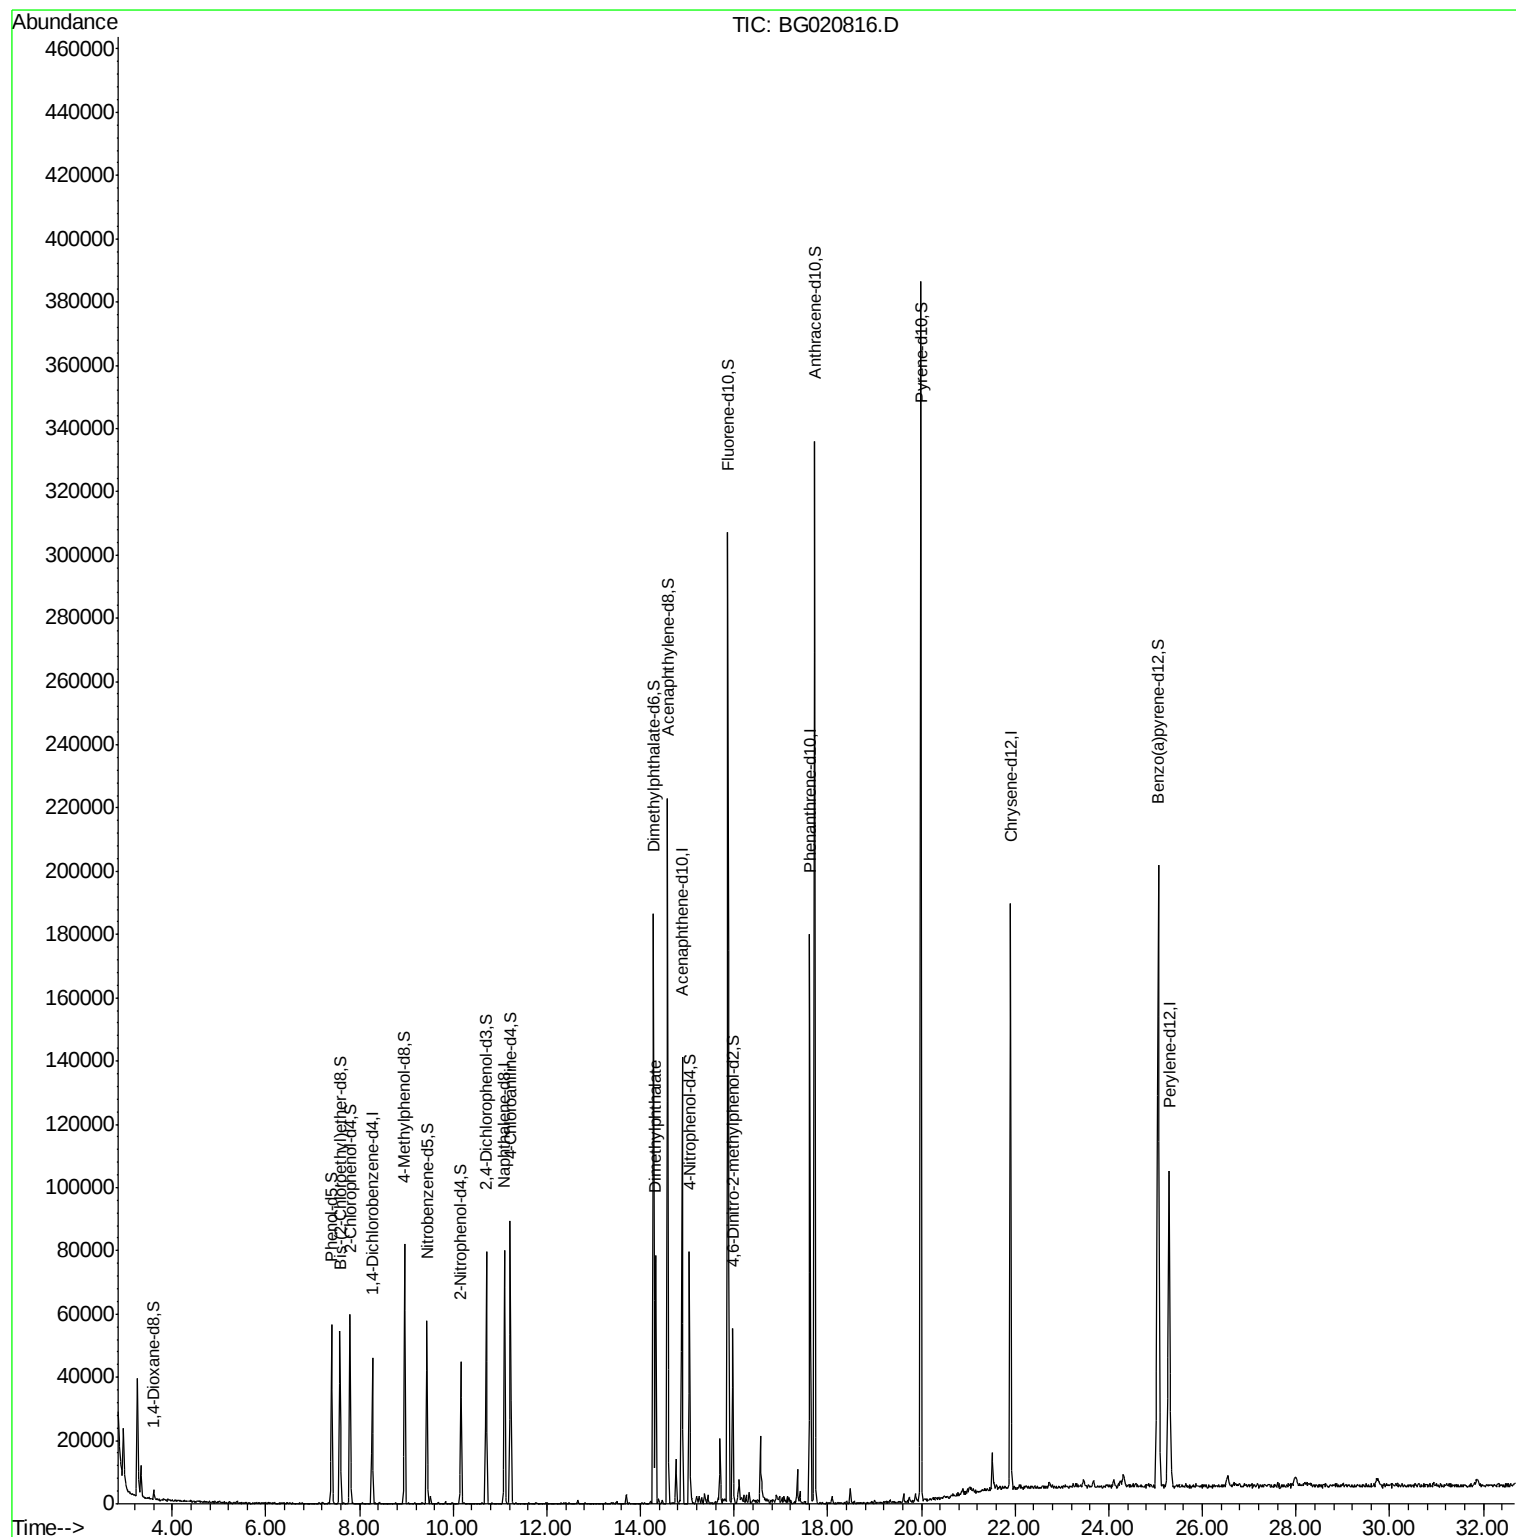

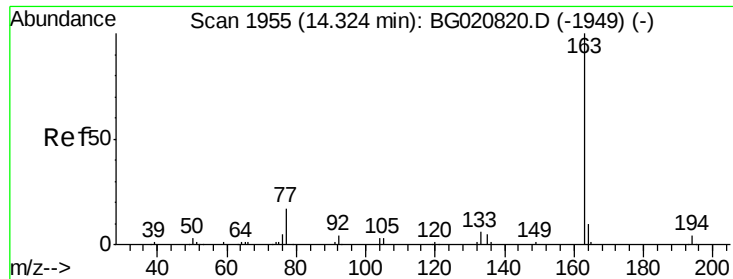

#45

Dimethylphthalate

Concen: 12.94 ng/ul

RT: 14.32 min Scan# 1955

Delta R.T. -0.01 min

Lab File: BG020816.D

Acq: 9 Feb 2016 14:11

Instrument :

BNA_G

ClientSampleId :

C04H9


Tot Ion:163 Resp: 56534

Ion Ratio Lower Upper

163 100

194 4.4 3.0 4.6

164 11.0 7.7 11.5

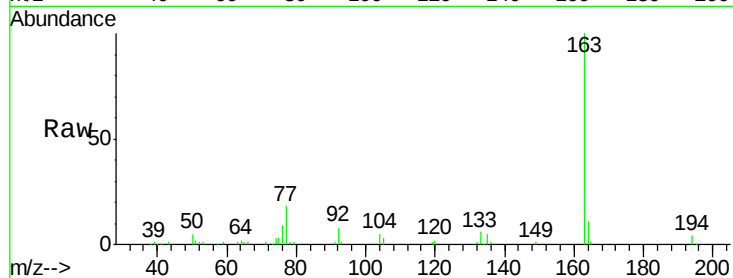

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

