


Data Path : Z:\HPCHEM1\BNA G\DATA\BG020916\
 Data File : BG020811.D
 Acq On : 9 Feb 2016 10:55
 Operator : SJ/UM
 Sample : DFTPP30
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP30

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG020816.M
 Title : SVOA CALIBRATION
 Last Update : Wed Feb 10 00:34:52 2016

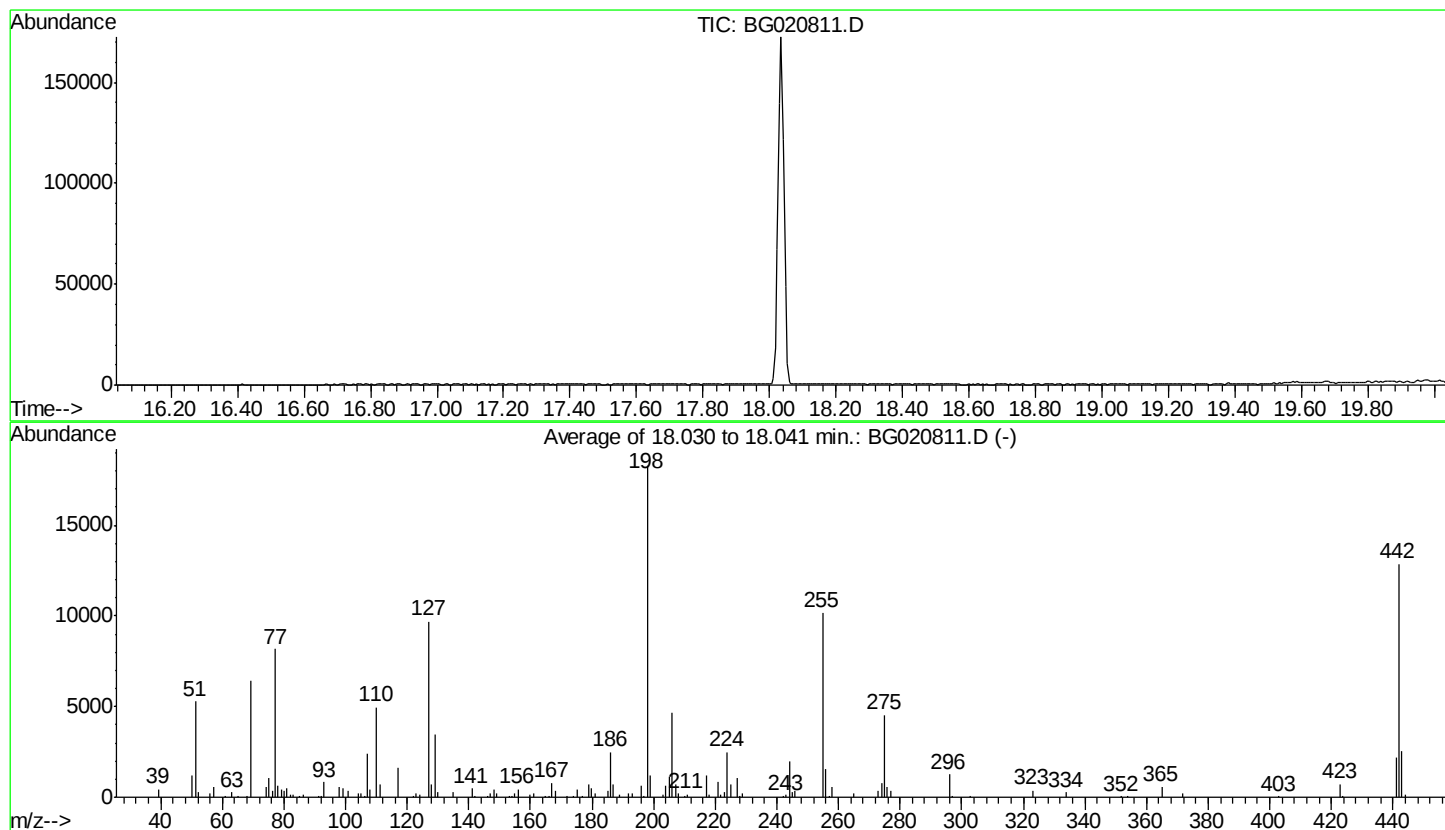

AutoFind: Scans 2586, 2587, 2588; Background Corrected with Scan 2581

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.9	5286	PASS
68	69	0.00	2	0.9	60	PASS
69	198	0.00	100	35.0	6400	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.1	9700	PASS
197	198	0.00	2	0.6	104	PASS
198	198	100	100	100.0	18284	PASS
199	198	5	9	6.6	1211	PASS
275	198	10	60	24.8	4537	PASS
365	198	1	100	3.1	565	PASS
441	442	0.01	100	17.1	2202	PASS
442	198	50	100	70.4	12877	PASS
443	442	15	24	19.8	2555	PASS

Scan 2581 (18.000 min): BG020811.D
DFTPP30

m/z	Abundance
40.05	221.0
44.15	171.0
123.05	199.0
149.05	250.0

Instrument :
BNA_G
ClientSampleId :
DFTPP30

m/z	Abundance
39.15	463.0
40.05	239.0
44.05	161.0
50.15	1450.0
51.15	5526.0
52.05	365.0
56.05	290.0
57.05	597.0
61.05	163.0
63.05	325.0
65.05	178.0
69.05	6746.0
74.05	669.0
75.05	1073.0
76.15	400.0
77.15	8664.0
78.05	535.0
79.05	492.0
80.05	397.0
81.05	579.0
82.05	163.0
82.95	182.0
84.95	201.0
86.05	245.0
93.05	879.0
98.05	613.0
99.05	570.0
101.05	375.0
103.95	249.0
105.05	194.0
107.05	2625.0
108.05	476.0
110.05	5176.0
111.05	814.0
117.05	1724.0
122.05	200.0
123.05	457.0
123.95	164.0
127.05	10414.0
127.95	755.0
129.05	3511.0
130.05	254.0
134.95	259.0
140.95	479.0
142.05	182.0
146.95	211.0
148.05	460.0
148.95	488.0
154.05	151.0
154.95	306.0
156.05	395.0
159.95	163.0
160.95	250.0
167.05	745.0
167.95	370.0
174.95	372.0
176.95	166.0
178.95	668.0
179.95	444.0
180.95	240.0
184.95	351.0
186.05	2522.0
186.95	810.0
191.95	226.0
192.95	248.0
195.95	602.0
197.95	17736.0
198.95	1099.0
202.95	162.0
204.05	683.0
204.95	1007.0
206.05	4619.0
207.05	597.0
208.05	207.0
210.05	157.0
210.85	239.0
216.95	1200.0
220.95	816.0
222.85	288.0
223.95	2420.0
224.95	562.0
226.95	1057.0
228.85	211.0
242.95	199.0
244.05	1875.0
244.95	330.0
245.95	294.0
254.95	9543.0
255.95	1521.0
257.95	408.0
264.85	207.0
272.95	274.0

Instrument :
BNA_G
ClientSampleId :
DFTPP30

273.95	644.0
274.95	3846.0
275.95	525.0
276.95	313.0
295.95	1139.0
322.95	262.0
333.95	251.0
364.95	428.0
371.85	203.0
422.95	496.0
440.95	1834.0
441.95	9538.0
442.95	1880.0

Instrument :
BNA_G
ClientSampleId :
DFTPP30

m/z	Abundance
39.05	523.0
40.05	196.0
50.15	1400.0
51.15	6133.0
52.15	303.0
56.05	251.0
57.05	614.0
63.05	282.0
68.05	181.0
69.05	7519.0
74.05	719.0
75.05	1222.0
76.15	399.0
77.15	9726.0
78.05	892.0
79.05	470.0
80.05	451.0
81.05	588.0
82.05	249.0
83.05	151.0
86.05	199.0
91.05	156.0
92.05	218.0
93.05	1039.0
98.05	706.0
99.05	529.0
100.95	390.0
104.05	187.0
104.95	289.0
106.05	158.0
107.05	2730.0
108.05	458.0
110.05	6071.0
111.05	879.0
117.05	1906.0
122.95	534.0
124.05	266.0
127.05	11449.0
128.05	856.0
129.05	4165.0
129.95	426.0
135.05	353.0
140.95	501.0
145.95	168.0
146.95	249.0
147.95	460.0
148.95	392.0
155.05	386.0
156.05	524.0
160.05	201.0
161.05	226.0
164.95	181.0
165.95	238.0
167.05	933.0
167.95	393.0
172.05	175.0
173.95	190.0
175.05	555.0
176.95	151.0
178.95	880.0
179.95	547.0
180.95	260.0
185.05	372.0
186.05	3039.0
187.05	778.0
188.95	175.0
191.95	268.0
192.95	265.0
195.95	772.0
196.85	313.0
197.95	21568.0
198.95	1492.0
202.95	169.0
204.05	774.0
205.05	1326.0
206.05	5653.0
207.05	869.0
207.95	244.0
210.95	231.0
216.95	1430.0
217.95	182.0
220.95	1000.0
221.95	224.0
222.95	397.0
224.05	2902.0
224.95	781.0
226.95	1265.0
227.95	183.0
228.95	259.0
241.95	155.0
243.95	2210.0
244.95	339.0

Instrument :
BNA_G
ClientSampleId :
DFTPP30

245.95	490.0
254.95	11901.0
255.95	1709.0
256.95	154.0
257.95	665.0
264.95	297.0
272.95	372.0
273.95	998.0
274.95	5725.0
275.95	705.0
276.95	372.0
295.95	1455.0
296.95	294.0
302.95	197.0
322.95	439.0
333.95	278.0
353.95	153.0
364.95	676.0
371.95	220.0
422.95	976.0
423.85	153.0
440.95	2434.0
441.95	15144.0
442.95	3022.0
443.85	273.0

Instrument :
BNA_G
ClientSampleId :
DFTPP30

m/z	Abundance
39.15	313.0
39.95	180.0
50.05	837.0
51.15	4201.0
52.15	178.0
57.05	441.0
63.05	167.0
69.05	4935.0
74.05	398.0
75.05	783.0
76.05	280.0
77.15	6087.0
78.05	412.0
79.05	363.0
80.05	240.0
81.05	347.0
82.95	154.0
93.05	612.0
98.05	451.0
98.95	358.0
101.05	244.0
103.95	228.0
105.05	195.0
107.05	1891.0
108.05	385.0
110.05	3615.0
111.05	458.0
117.05	1260.0
123.05	337.0
127.05	7237.0
128.05	601.0
129.05	2638.0
129.95	186.0
134.95	234.0
140.95	420.0
146.95	213.0
147.95	422.0
149.05	410.0
153.05	177.0
155.95	397.0
160.95	223.0
167.05	749.0
168.05	305.0
175.05	329.0
178.95	624.0
179.95	413.0
180.95	158.0
184.95	244.0
185.95	1940.0
187.05	606.0
189.05	161.0
191.95	170.0
192.95	222.0
195.95	454.0
197.95	15548.0
198.95	1044.0
203.95	561.0
204.95	1028.0
206.05	3798.0
207.05	595.0
208.05	160.0
216.95	1016.0
217.95	155.0
220.95	835.0
221.85	179.0
222.95	239.0
224.05	2193.0
225.05	694.0
226.95	857.0
228.95	180.0
243.05	183.0
243.95	1795.0
244.95	241.0
245.95	315.0
254.95	9115.0
255.95	1473.0
257.95	524.0
264.95	230.0
272.95	350.0
273.95	770.0
274.95	4042.0
275.95	544.0
276.95	391.0
295.95	1195.0
322.95	368.0
333.95	266.0
351.85	156.0
364.95	591.0
371.95	191.0
402.95	170.0
422.95	754.0
440.95	2339.0

Instrument :
BNA_G
ClientSampleId :
DFTPP30

441.95	13950.0
442.95	2765.0
443.95	187.0

Instrument :
BNA_G
ClientSampleId :
DFTPP30