
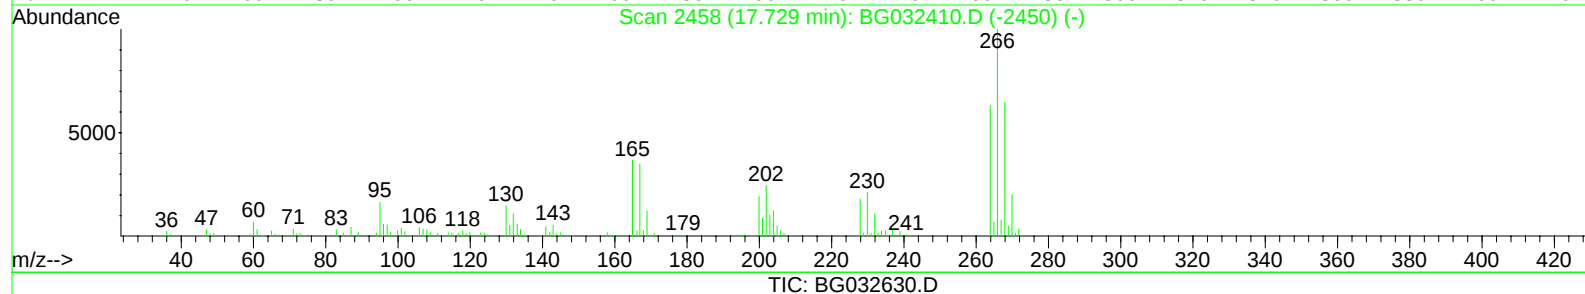
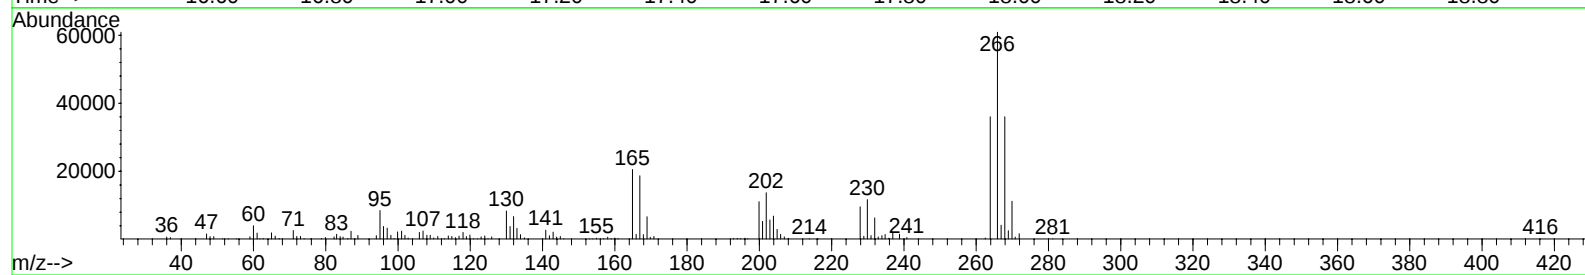


Data Path : Z:\HPCHEM1\BNA G\DATA\BG020918\
Data File : BG032630.D
Acq On : 9 Feb 2018 12:46
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 10 00:36:26 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 18:57:08 2018
Response via : Initial Calibration

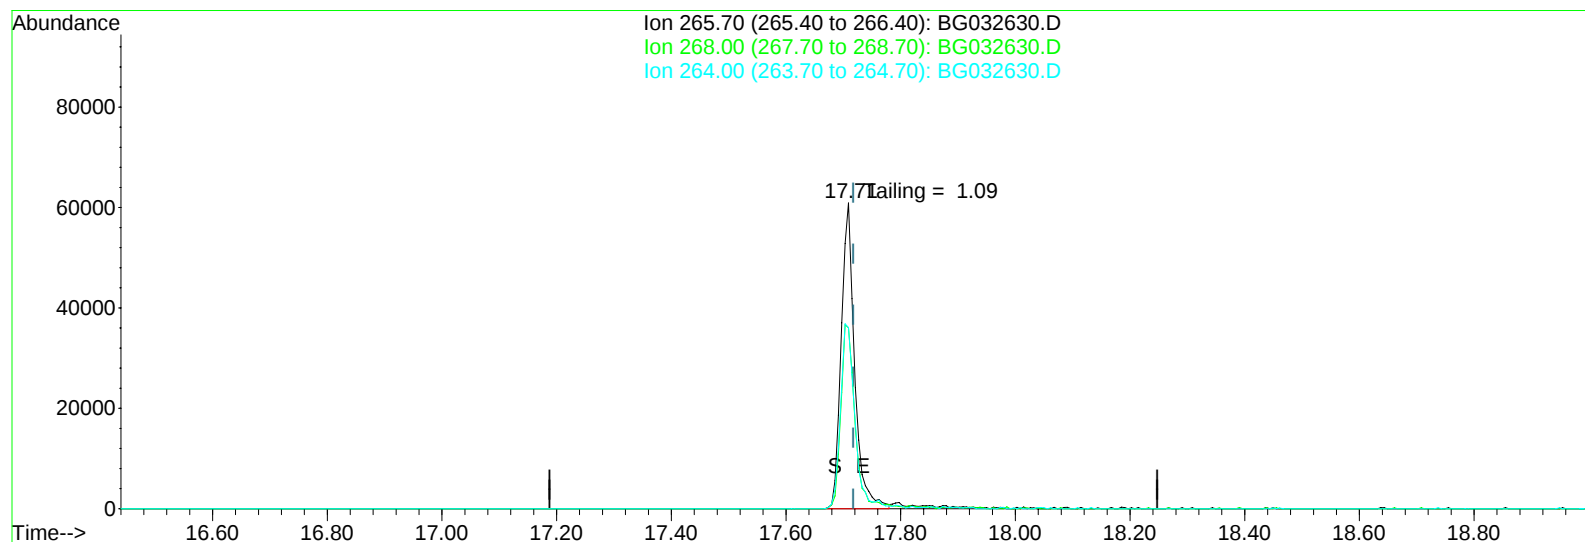

(69) Pentachlorophenol (C)




17.709min (-0.008) 174276.30ng

response 98444

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.17
264.00	62.00	59.19
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG020918\
Data File : BG032630.D
Acq On : 9 Feb 2018 12:46
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 10 00:36:26 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG012918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 06 18:57:08 2018
Response via : Initial Calibration

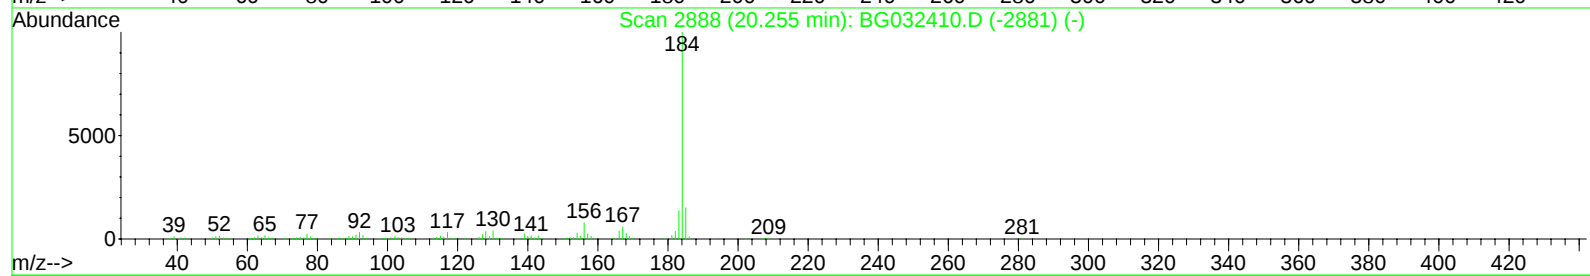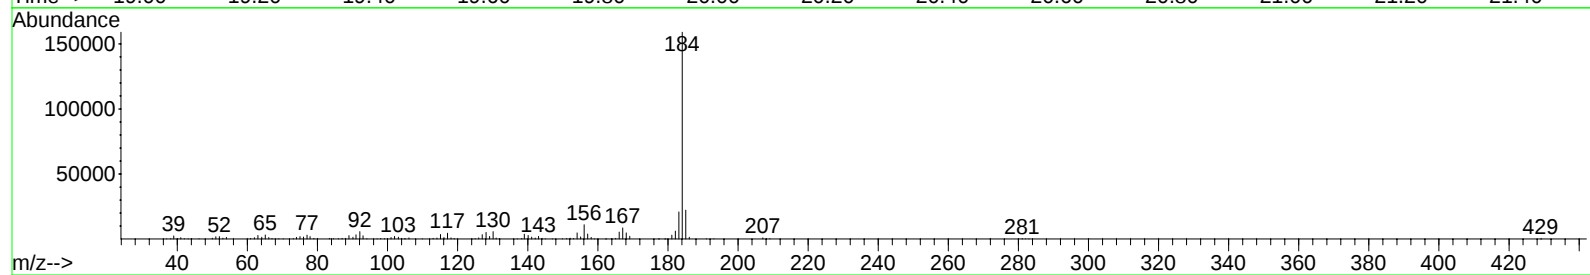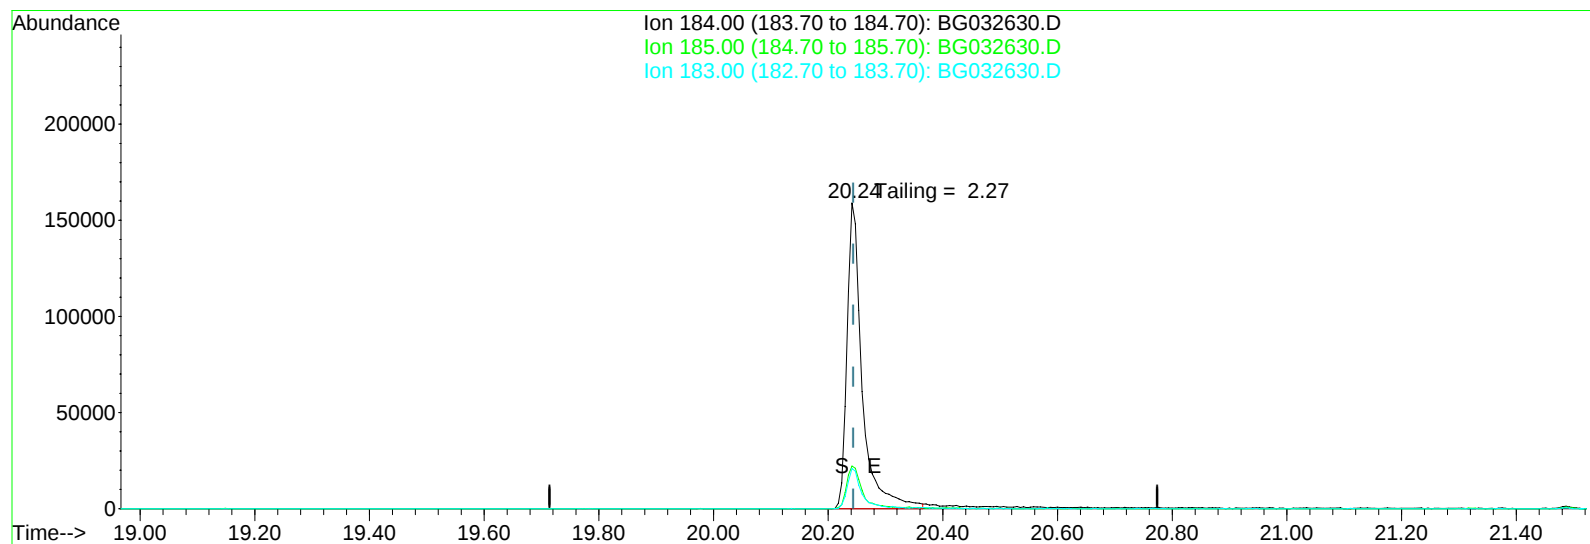

TIC: BG032630.D

(76) Benzidine

20.241min (-0.002) 259259.89ng

response 295268

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.94
183.00	13.30	13.11
0.00	0.00	0.00