


Data Path : Z:\HPCHEM1\BNA G\Data\BG020918\
 Data File : BG032630.D
 Acq On : 9 Feb 2018 12:46
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG012918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 06 18:57:08 2018

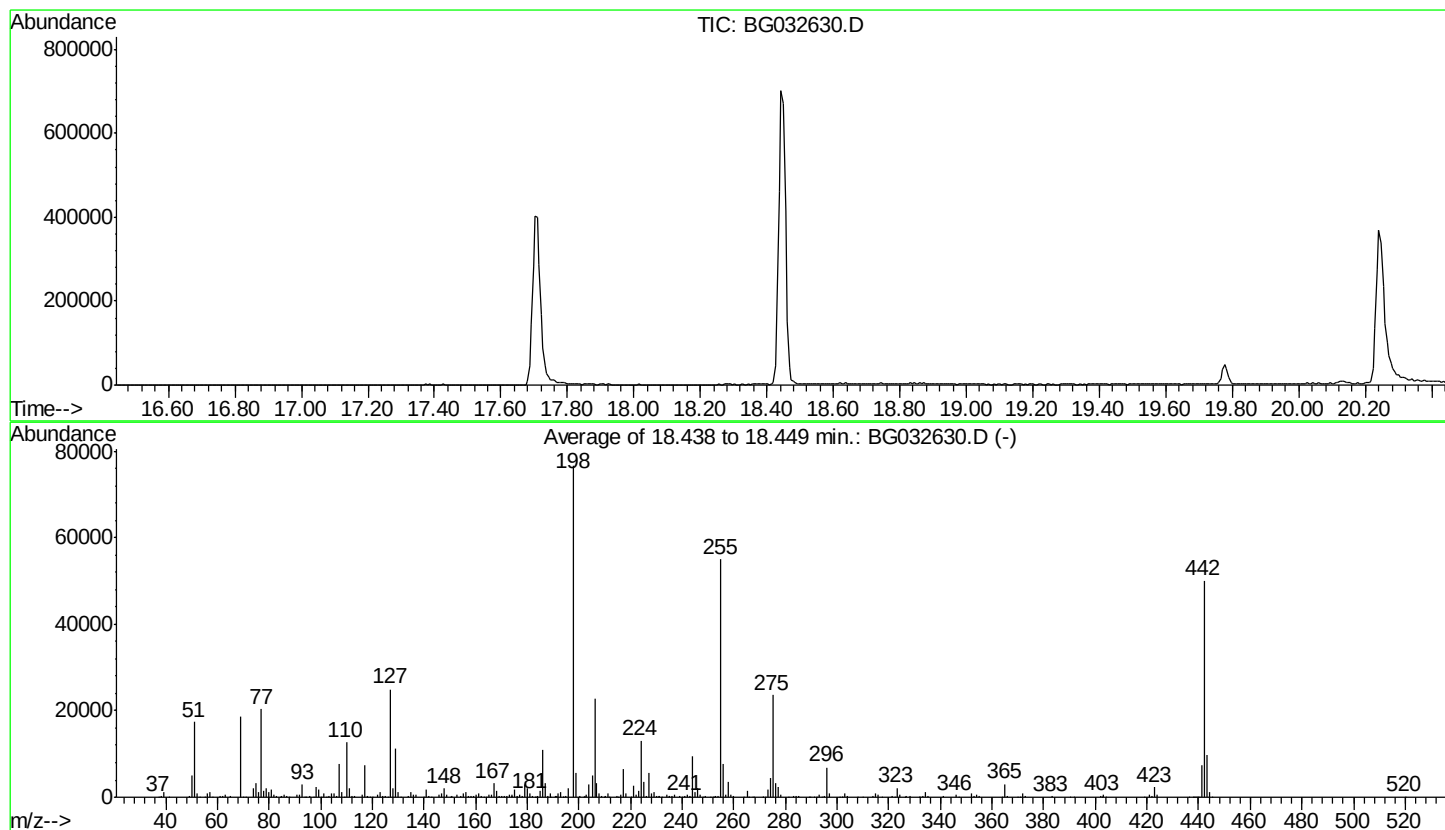

AutoFind: Scans 2578, 2579, 2580; Background Corrected with Scan 2571

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	22.7	17440	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	24.2	18541	PASS
70	69	0.00	2	0.8	154	PASS
127	198	10	80	32.6	24986	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	76685	PASS
199	198	5	9	7.3	5602	PASS
275	198	10	60	30.7	23560	PASS
365	198	1	100	3.9	2973	PASS
441	442	0.01	24	14.6	7338	PASS
442	198	50	100	65.3	50096	PASS
443	442	15	24	19.7	9866	PASS