
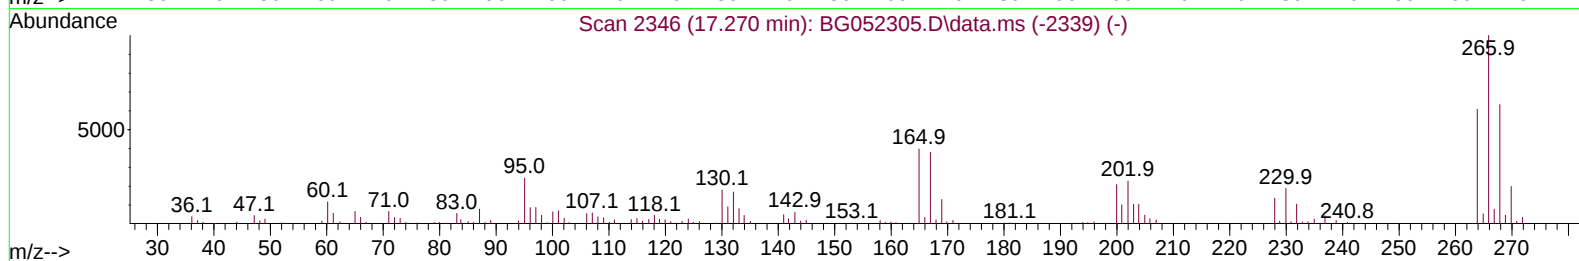
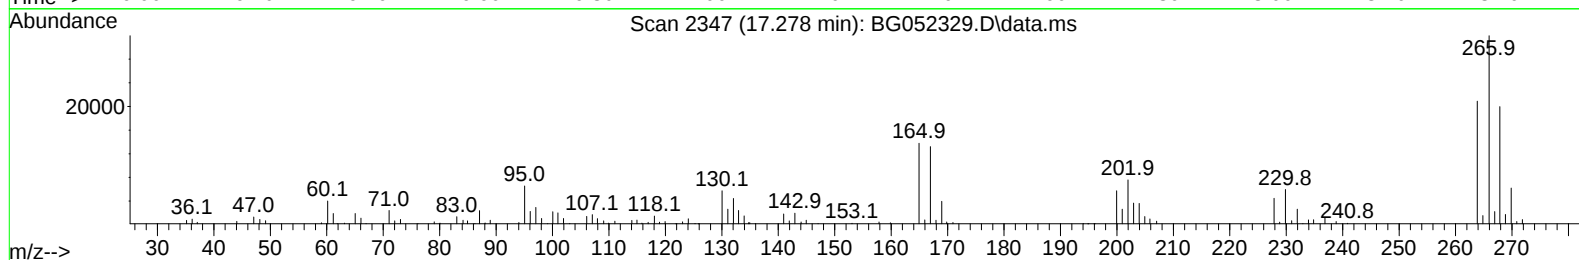


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG020922\  
Data File : BG052329.D  
Acq On : 9 Feb 2022 10:37  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 09 11:42:37 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG020722.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Feb 08 01:21:20 2022  
Response via : Initial Calibration

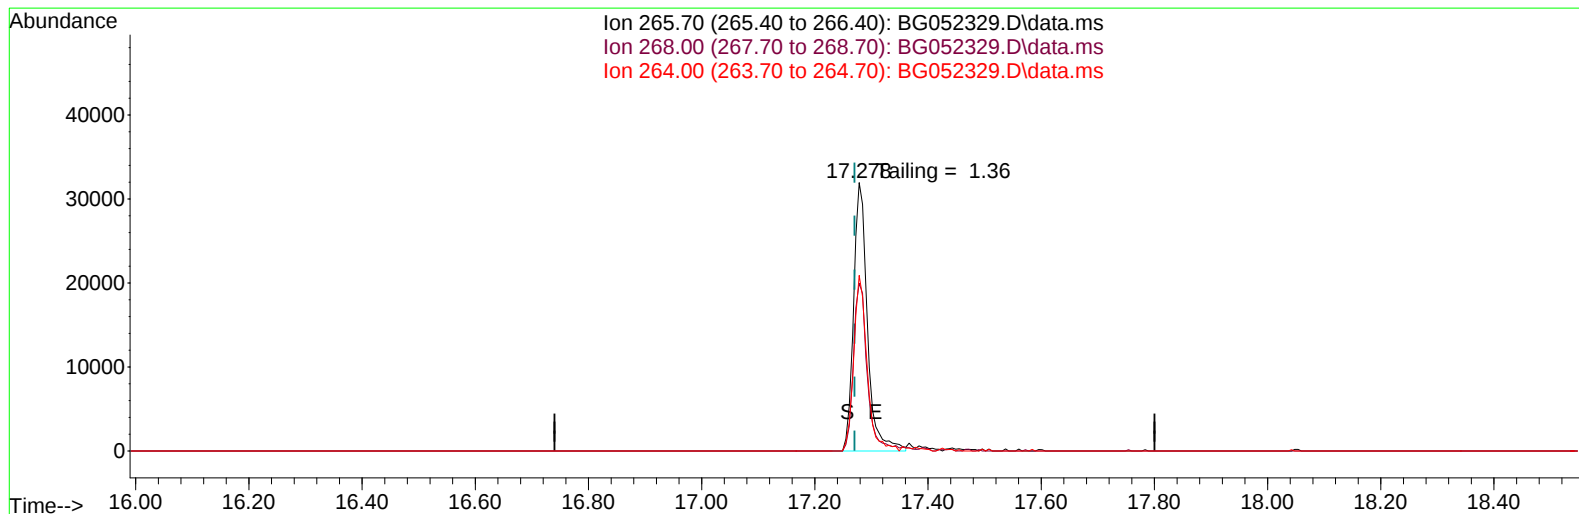

TIC: BG052329.D\data.ms

**(70) Pentachlorophenol (C)**




17.278min (+ 0.008) 22962.35 ng

response 54231

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.20  | 62.46  |
| 264.00 | 65.20  | 65.41  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG020922\  
 Data File : BG052329.D  
 Acq On : 9 Feb 2022 10:37  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 09 11:42:37 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG020722.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Feb 08 01:21:20 2022  
 Response via : Initial Calibration

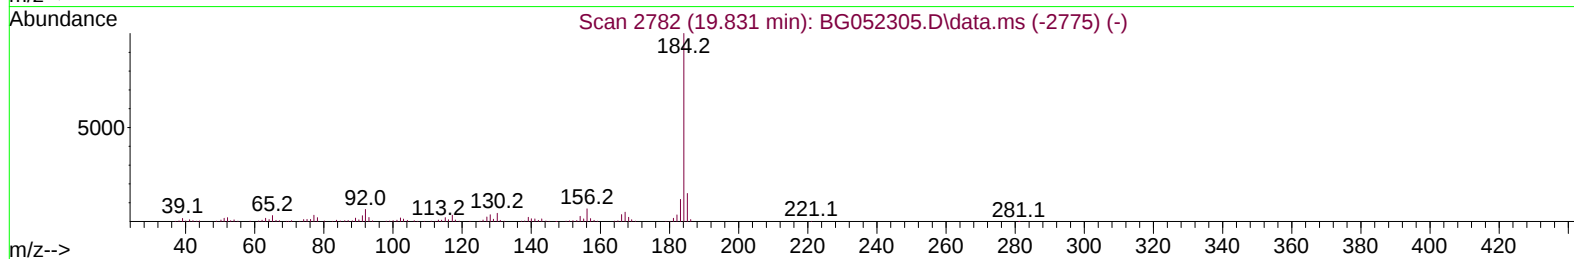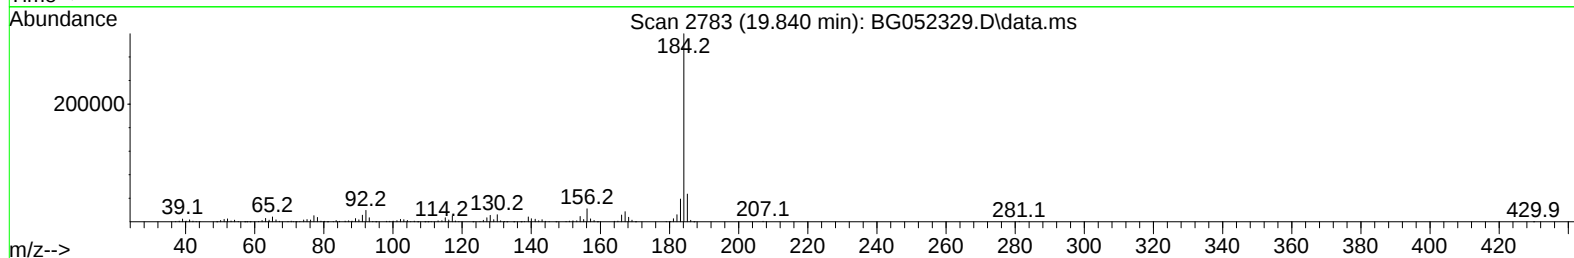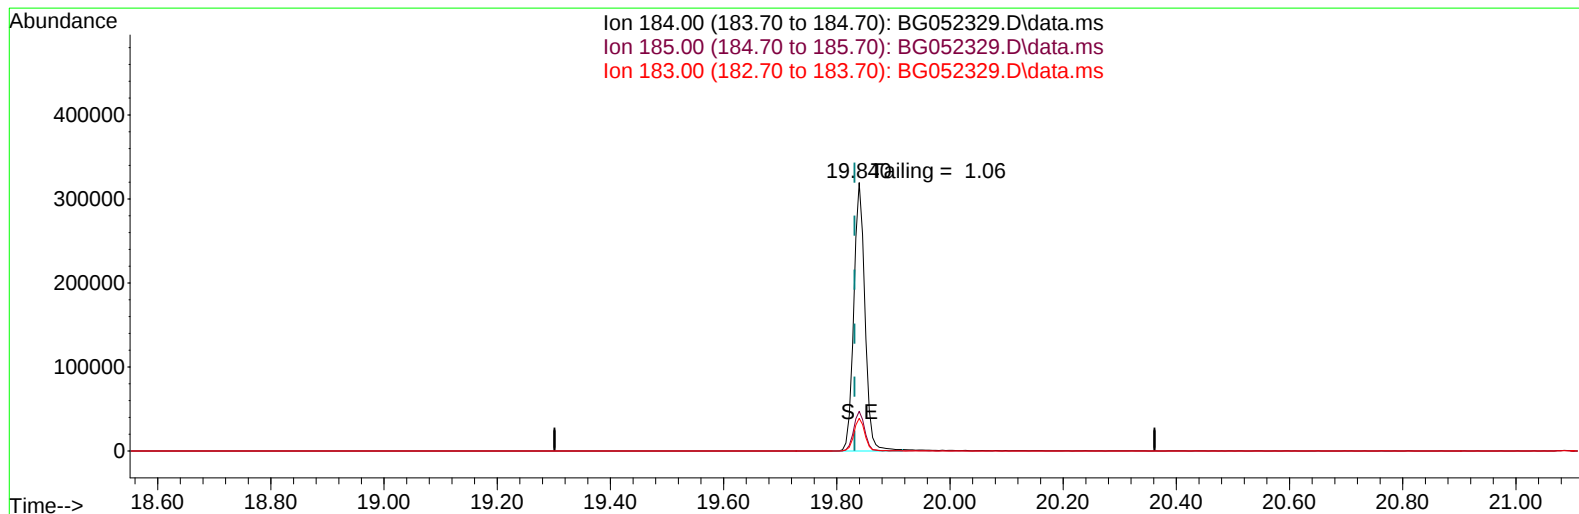

TIC: BG052329.D\data.ms

**(77) Benzidine**

19.840min (+ 0.009) 349965.80 ng m

response 433723

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.80  | 14.79  |
| 183.00 | 12.20  | 12.17  |
| 0.00   | 0.00   | 0.00   |