

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020922\
 Data File : BG052336.D
 Acq On : 9 Feb 2022 15:48
 Operator : CG/JU
 Sample : N1423-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP-21

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG052336.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.756	376	386	396	rBV	374783	603205	33.52%	7.405%
2	7.377	654	662	671	rBV	394010	704300	39.14%	8.646%
3	8.229	799	807	813	rBV	92895	158778	8.82%	1.949%
4	9.398	998	1006	1018	rBV	251381	453026	25.18%	5.561%
5	11.066	1283	1290	1305	rVB	131878	239903	13.33%	2.945%
6	13.498	1696	1704	1711	rVB	715200	1094818	60.84%	13.439%
7	14.873	1931	1938	1945	rVB	234845	373300	20.75%	4.582%
8	16.359	2185	2191	2201	rBV	631871	943406	52.43%	11.581%
9	17.622	2399	2406	2411	rBV	326523	497509	27.65%	6.107%
10	17.669	2411	2414	2421	rVB2	21067	31142	1.73%	0.382%
11	18.486	2549	2553	2559	rBV5	12925	21835	1.21%	0.268%
12	19.666	2750	2754	2762	rVB	27593	42869	2.38%	0.526%
13	20.031	2810	2816	2822	rVB	23535	38228	2.12%	0.469%
14	20.219	2842	2848	2853	rBV	1373867	1799395	100.00%	22.088%
15	21.534	3067	3072	3079	rBV3	39724	65350	3.63%	0.802%
16	21.940	3133	3141	3147	rBV	309628	540774	30.05%	6.638%
17	25.417	3722	3733	3746	rVB	175531	538573	29.93%	6.611%




Sum of corrected areas: 8146411

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020922\
Data File : BG052336.D
Acq On : 9 Feb 2022 15:48
Operator : CG/JU
Sample : N1423-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-21

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

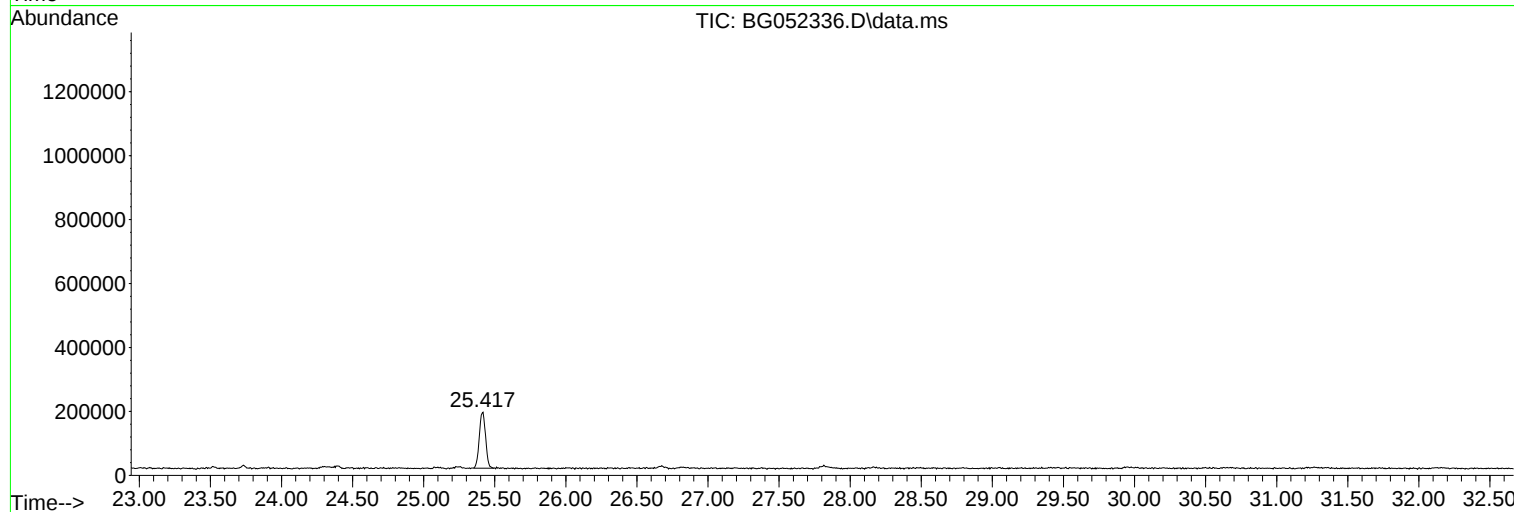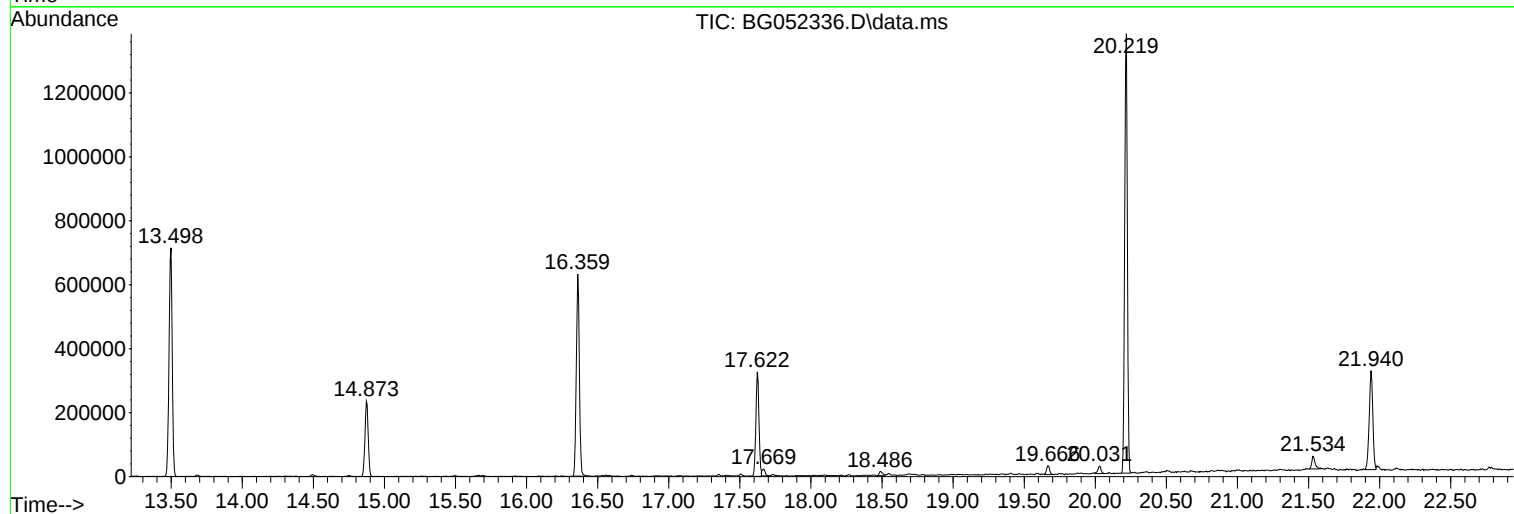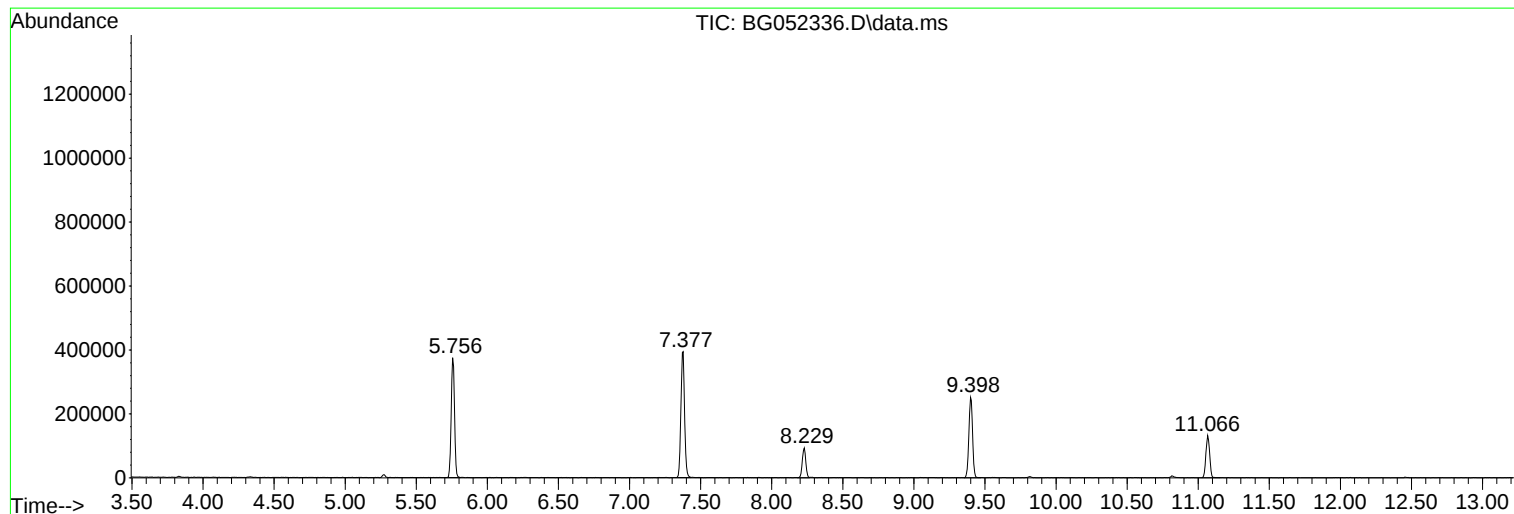

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020922\
Data File : BG052336.D
Acq On : 9 Feb 2022 15:48
Operator : CG/JU
Sample : N1423-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-21










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Cyclopentadecane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.535	2.42 ng	65350	Chrysene-d12	21.940

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopentadecane	210	C15H30	000295-48-7	97
2			E-2-Hexadecacen-1-ol	240	C16H32O	1010131-10-1	96
3			Cyclotetradecane	196	C14H28	000295-17-0	95
4			Dichloroacetic acid, heptadecyl ...	366	C19H36Cl2O2	1000282-98-2	95
5			Trifluoroacetic acid, pentadecyl...	324	C17H31F3O2	959010-23-2	94

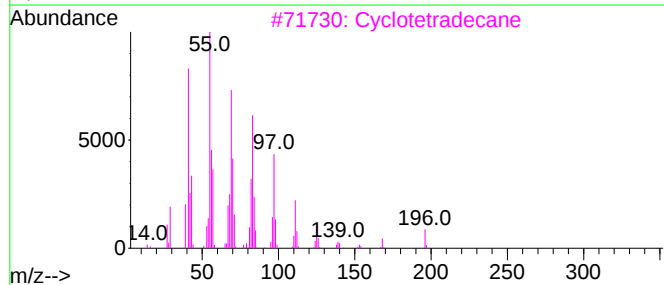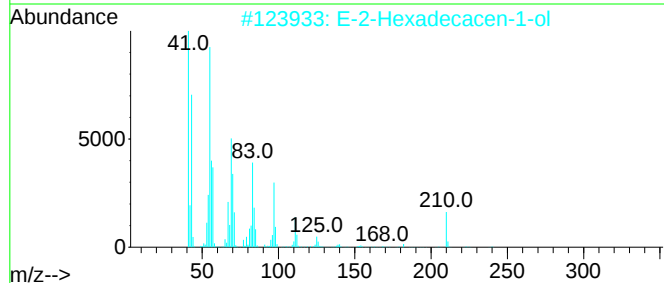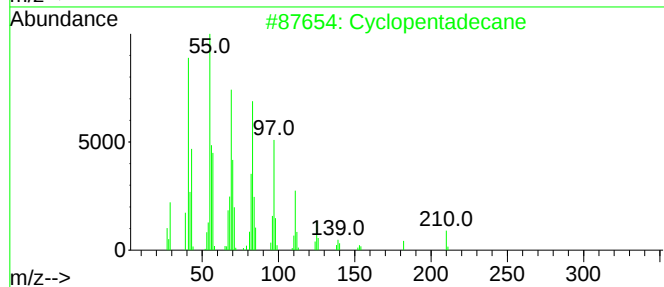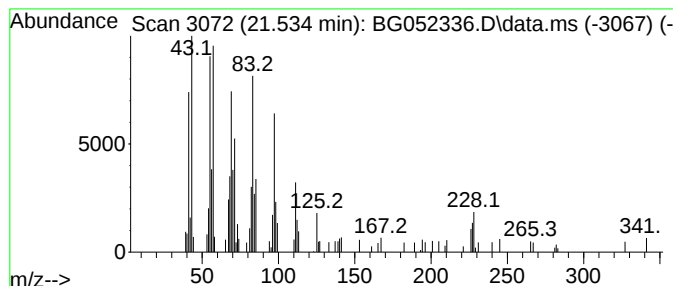

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020922\
Data File : BG052336.D
Acq On : 9 Feb 2022 15:48
Operator : CG/JU
Sample : N1423-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-21

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Cyclopentadecane	21.535	2.4	ng	65350	5	21.940	540774	20.0