

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020922\
 Data File : BG052338.D
 Acq On : 9 Feb 2022 17:05
 Operator : CG/JU
 Sample : N1423-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP-23

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG052338.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.756	379	386	397	rBV	313551	506593	31.95%	7.025%
2	7.372	654	661	673	rBV	328707	581093	36.65%	8.058%
3	8.223	800	806	814	rBV	88053	151019	9.52%	2.094%
4	9.398	997	1006	1015	rBV	212740	376284	23.73%	5.218%
5	11.067	1283	1290	1301	rBV	125980	226269	14.27%	3.138%
6	13.493	1696	1703	1711	rBV	598849	920047	58.02%	12.759%
7	14.873	1932	1938	1945	rVB	230737	358040	22.58%	4.965%
8	16.359	2184	2191	2204	rBV	536408	816073	51.46%	11.317%
9	17.622	2400	2406	2412	rBV	329577	480747	30.32%	6.667%
10	18.486	2549	2553	2560	rBV4	19242	26861	1.69%	0.372%
11	20.219	2840	2848	2853	rBV	1187954	1585722	100.00%	21.990%
12	21.006	2977	2982	2986	rBV6	10974	16325	1.03%	0.226%
13	21.535	3068	3072	3081	rVB2	39576	63516	4.01%	0.881%
14	21.940	3134	3141	3151	rVB2	298508	506693	31.95%	7.026%
15	22.122	3167	3172	3176	rBV4	14464	24710	1.56%	0.343%
16	22.768	3279	3282	3292	rVB8	14724	25693	1.62%	0.356%
17	23.520	3406	3410	3417	rVB6	11761	23465	1.48%	0.325%
18	25.418	3721	3733	3746	rVB2	163994	522074	32.92%	7.240%




Sum of corrected areas: 7211224

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020922\
Data File : BG052338.D
Acq On : 9 Feb 2022 17:05
Operator : CG/JU
Sample : N1423-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-23

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

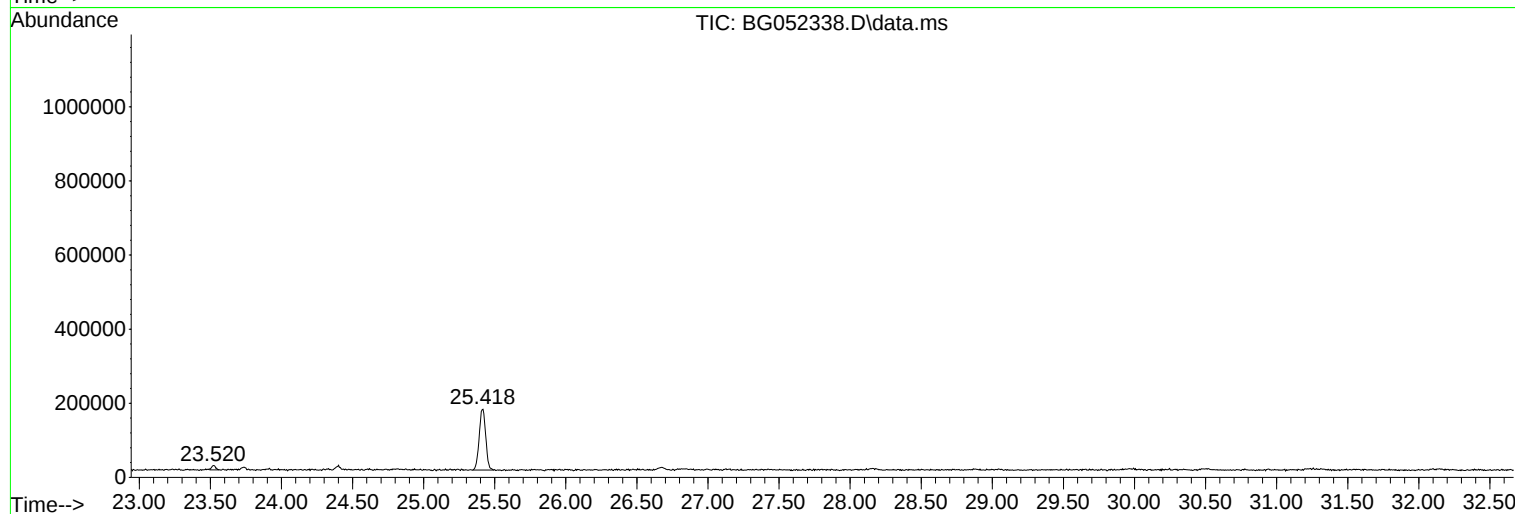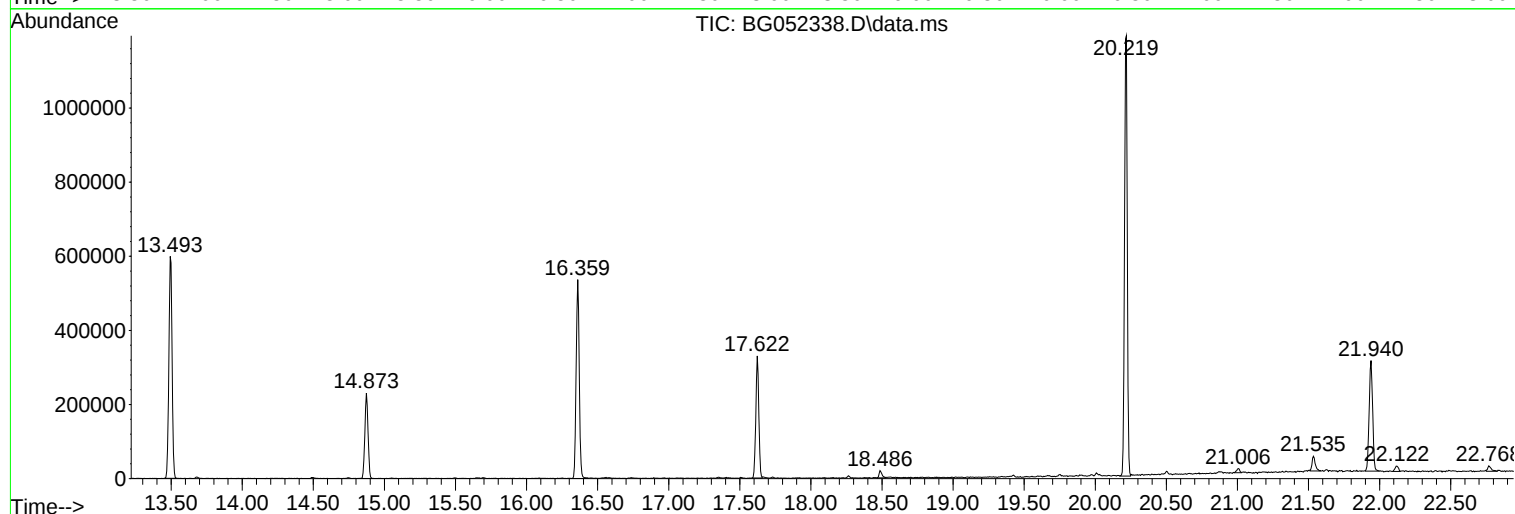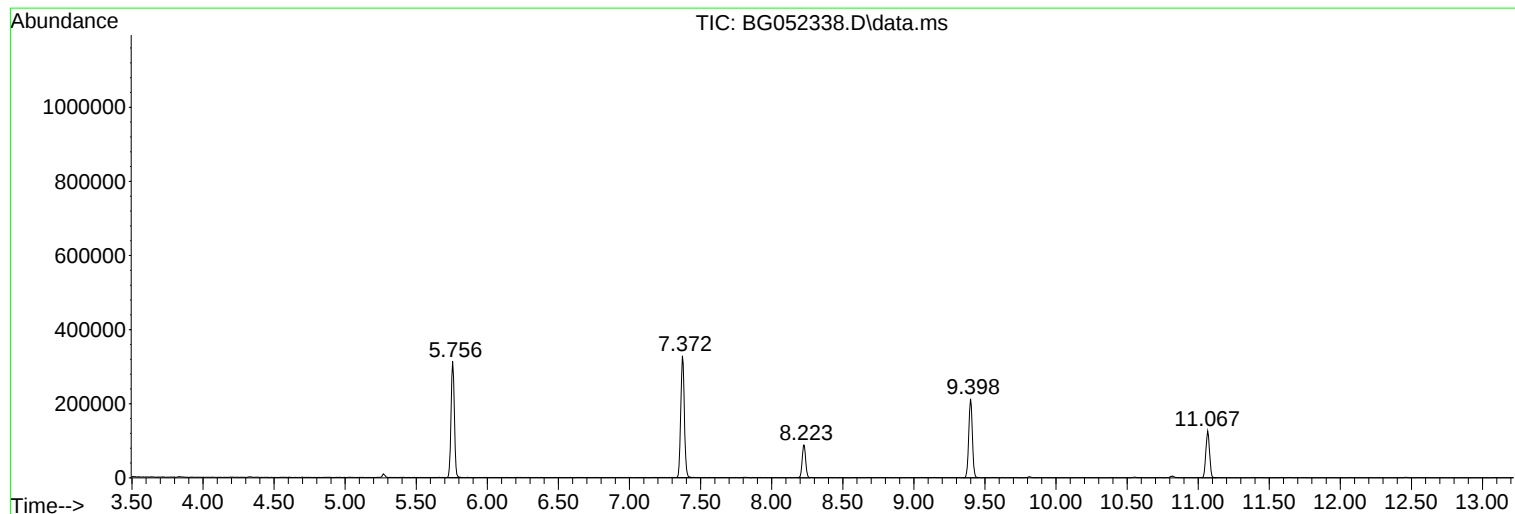

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020922\
Data File : BG052338.D
Acq On : 9 Feb 2022 17:05
Operator : CG/JU
Sample : N1423-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-23










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Octatriacontyl pentafluorop... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.535	2.51 ng	63516	Chrysene-d12	21.940

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Octatriacontyl pentafluoropropio...	697	C41H77F5O2	1000351-89-1	91
2			1-Decanol, 2-octyl-	270	C18H38O	045235-48-1	91
3			Oxalic acid, isobutyl hexadecyl ...	370	C22H42O4	1000309-38-1	90
4			Oxalic acid, isobutyl octadecyl ...	398	C24H46O4	1000309-38-3	90
5			Oxalic acid, isobutyl pentadecyl...	356	C21H40O4	1000309-38-0	90

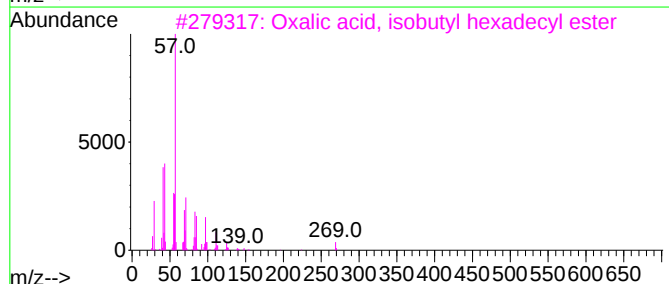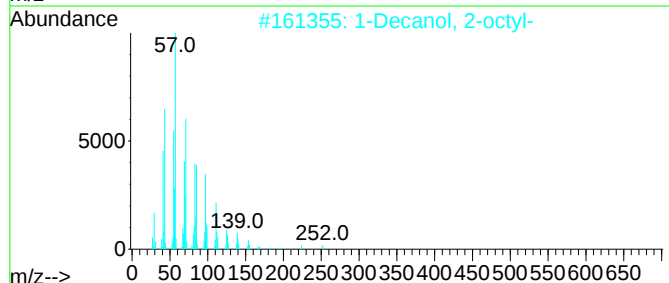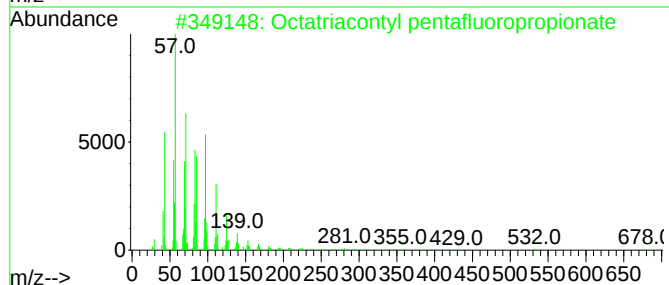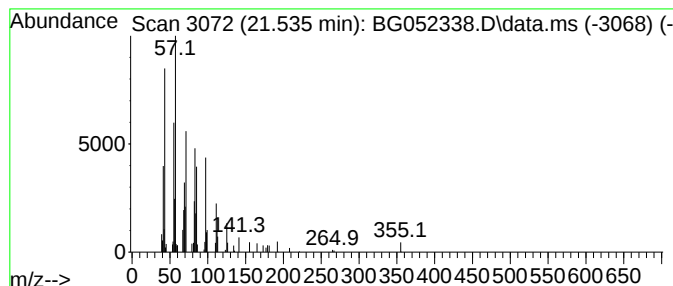

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020922\
Data File : BG052338.D
Acq On : 9 Feb 2022 17:05
Operator : CG/JU
Sample : N1423-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-23

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Octatriacontyl ...	21.535	2.5	ng	63516	5	21.940	506693	20.0