

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020922\
 Data File : BG052339.D
 Acq On : 9 Feb 2022 17:43
 Operator : CG/JU
 Sample : N1423-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP-24

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG052339.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.269	297	303	311	rBV	40848	59815	2.98%	0.725%
2	5.756	378	386	396	rBV	382746	611789	30.43%	7.413%
3	7.372	653	661	672	rBV	413963	704444	35.04%	8.536%
4	8.229	797	807	813	rBV	87020	151673	7.55%	1.838%
5	9.398	996	1006	1014	rBV	254084	453649	22.57%	5.497%
6	11.067	1282	1290	1301	rBV	132009	228515	11.37%	2.769%
7	13.493	1695	1703	1712	rBV	710725	1121059	55.77%	13.584%
8	14.873	1932	1938	1948	rVB	234882	359794	17.90%	4.360%
9	16.219	2162	2167	2173	rBV5	13947	20489	1.02%	0.248%
10	16.360	2184	2191	2202	rBV	637697	970300	48.27%	11.757%
11	17.623	2398	2406	2417	rBV	307572	489636	24.36%	5.933%
12	20.219	2841	2848	2855	rBV	1533782	2010222	100.00%	24.357%
13	21.535	3067	3072	3080	rBV4	28518	48435	2.41%	0.587%
14	21.940	3135	3141	3148	rVB	293999	504877	25.12%	6.117%
15	25.412	3722	3732	3744	rVB	167744	518394	25.79%	6.281%




Sum of corrected areas: 8253091

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020922\
Data File : BG052339.D
Acq On : 9 Feb 2022 17:43
Operator : CG/JU
Sample : N1423-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-24

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

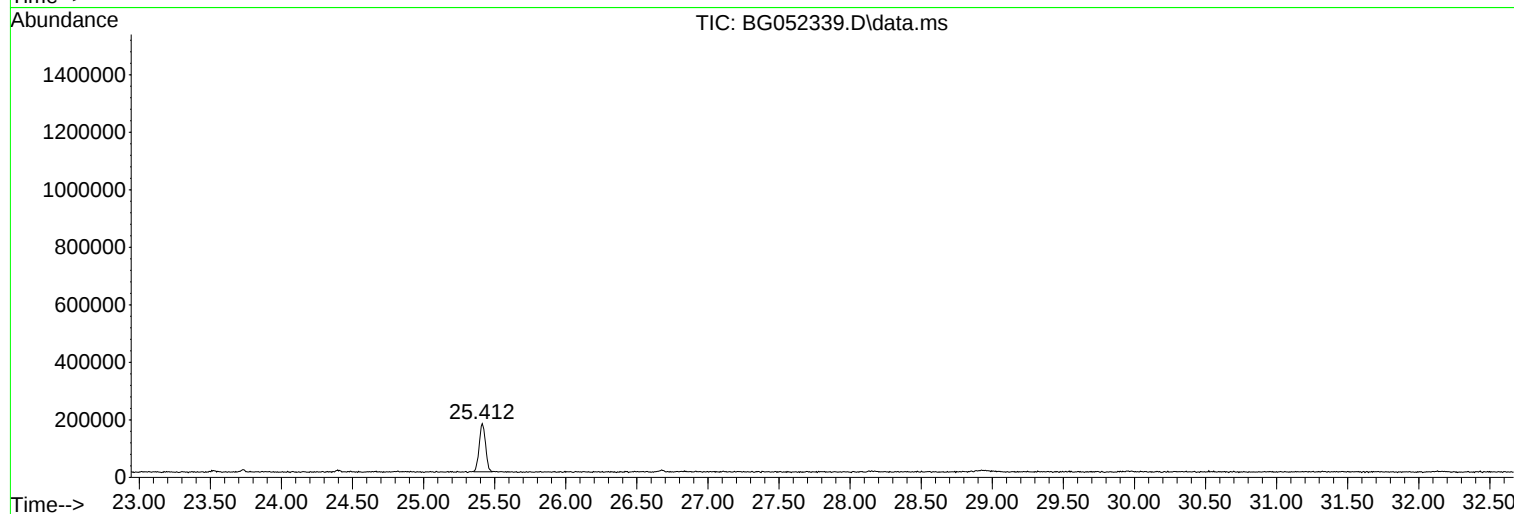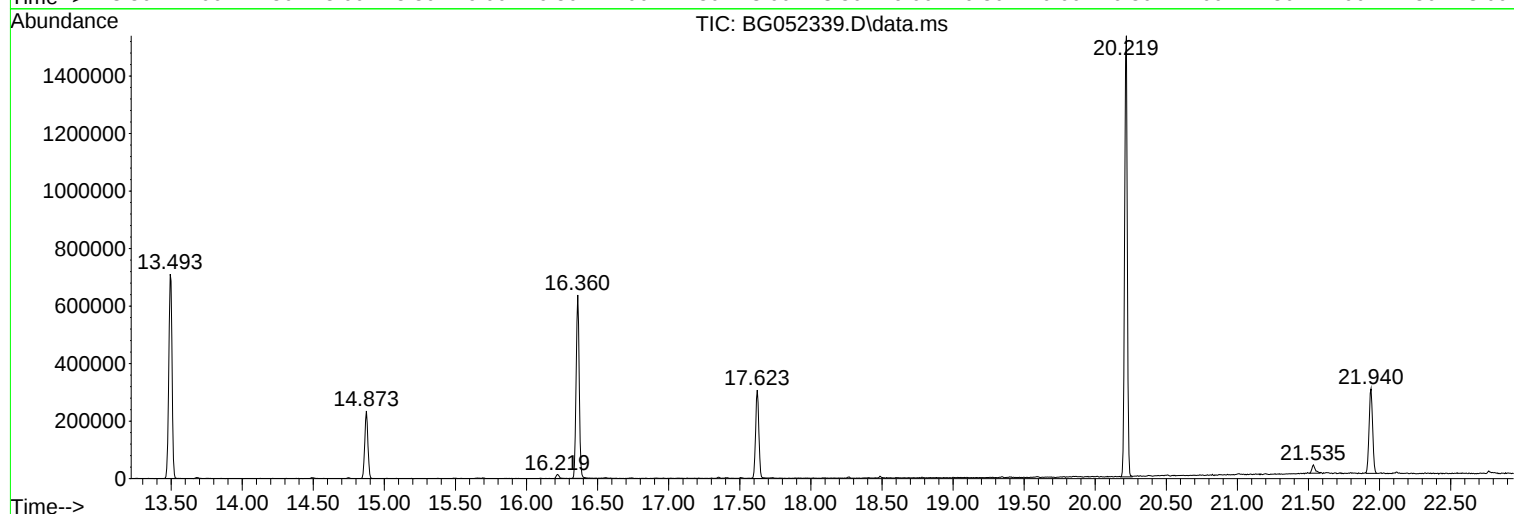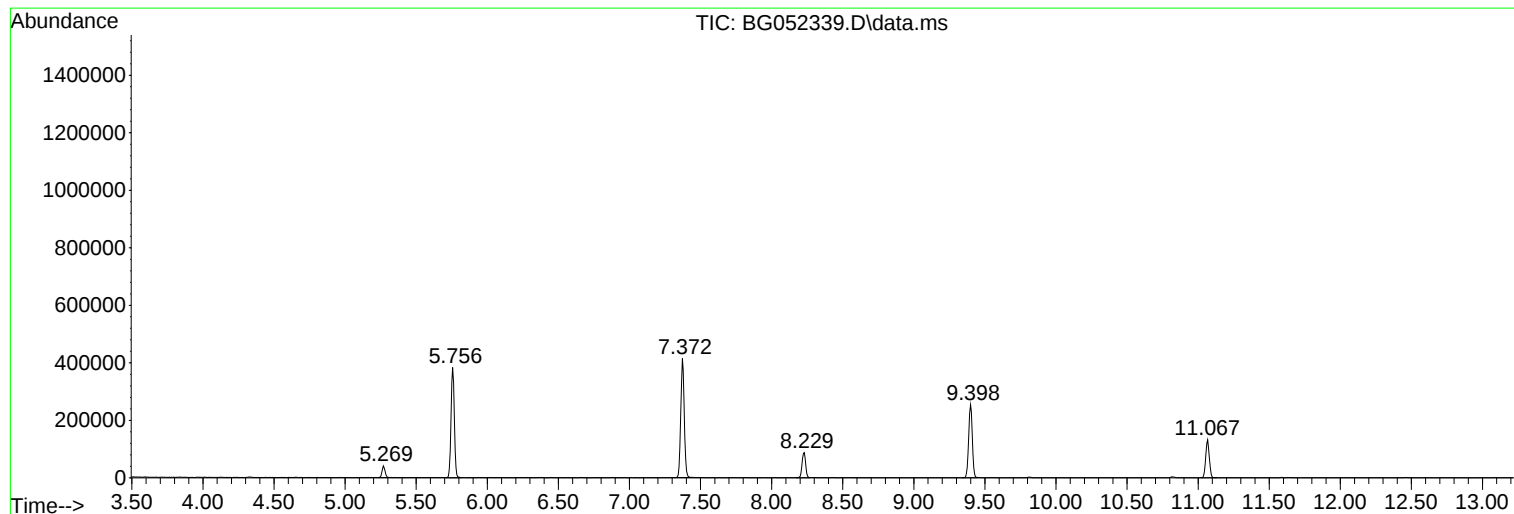

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020922\
Data File : BG052339.D
Acq On : 9 Feb 2022 17:43
Operator : CG/JU
Sample : N1423-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-24










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.269	7.89 ng	59815	1,4-Dichlorobenzene-d4	8.224

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64		
2	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	25		
3	3-Octanol	130	C8H18O	000589-98-0	23		
4	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	12		
5	2-Heptanone, 7,7-dichloro-	182	C7H12Cl2O	066241-43-8	10		

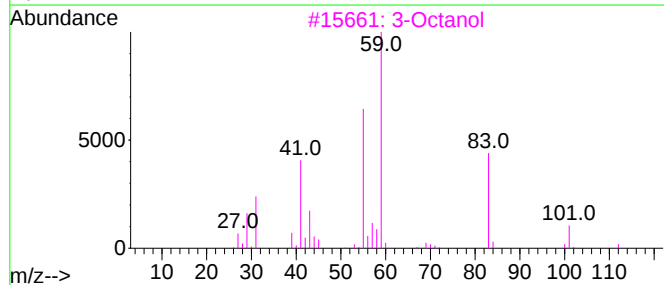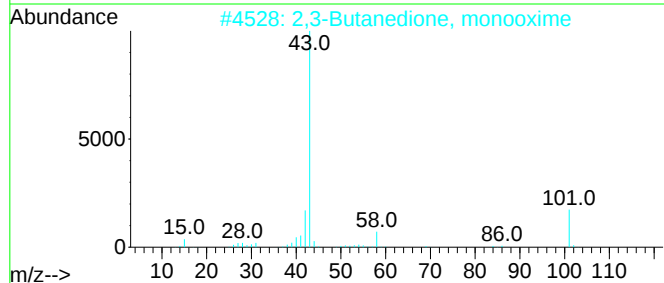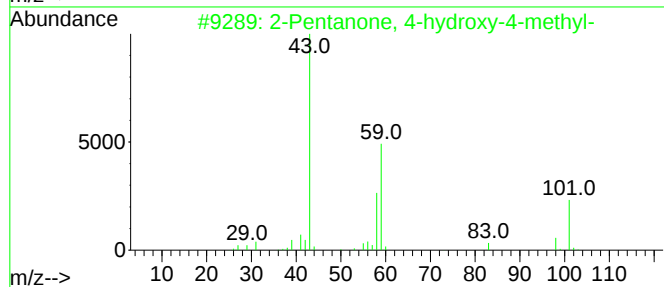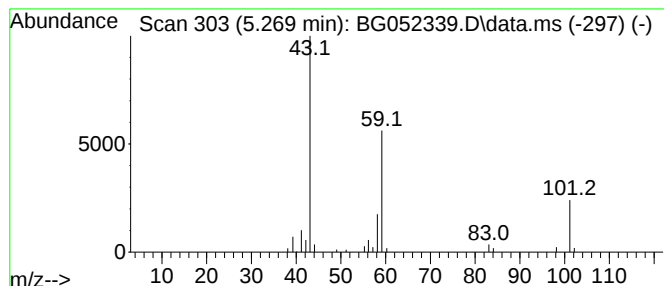

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020922\
Data File : BG052339.D
Acq On : 9 Feb 2022 17:43
Operator : CG/JU
Sample : N1423-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-24

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.269	7.9	ng	59815	1	8.224	151673	20.0