

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020922\
 Data File : BG052341.D
 Acq On : 9 Feb 2022 19:00
 Operator : CG/JU
 Sample : N1432-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SP-3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG052341.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.755	379	386	396	rBV	328895	525178	29.55%	7.040%
2	7.371	652	661	673	rBV	353627	620613	34.92%	8.319%
3	8.229	798	807	813	rBV	86458	144137	8.11%	1.932%
4	9.398	998	1006	1015	rBV	226500	402000	22.62%	5.389%
5	11.066	1283	1290	1298	rBV	119964	212758	11.97%	2.852%
6	13.492	1696	1703	1714	rBV	634688	991420	55.78%	13.290%
7	14.872	1932	1938	1948	rVB	228962	344517	19.38%	4.618%
8	16.359	2184	2191	2199	rBV	554120	859481	48.35%	11.521%
9	17.622	2398	2406	2412	rBV	311200	471880	26.55%	6.325%
10	20.218	2842	2848	2855	rBV	1364448	1777488	100.00%	23.827%
11	21.534	3067	3072	3080	rBV2	54865	92186	5.19%	1.236%
12	21.939	3134	3141	3148	rBV	290156	498326	28.04%	6.680%
13	25.411	3721	3732	3741	rBV2	172017	520009	29.26%	6.971%




Sum of corrected areas: 7459993

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020922\
Data File : BG052341.D
Acq On : 9 Feb 2022 19:00
Operator : CG/JU
Sample : N1432-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SP-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

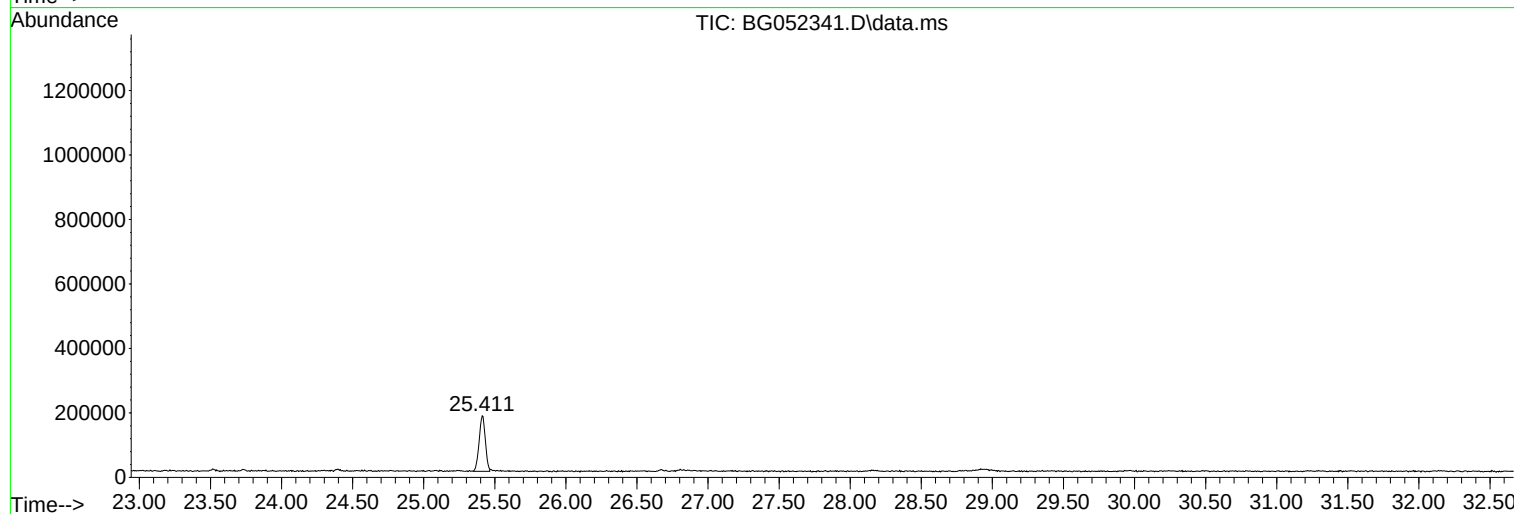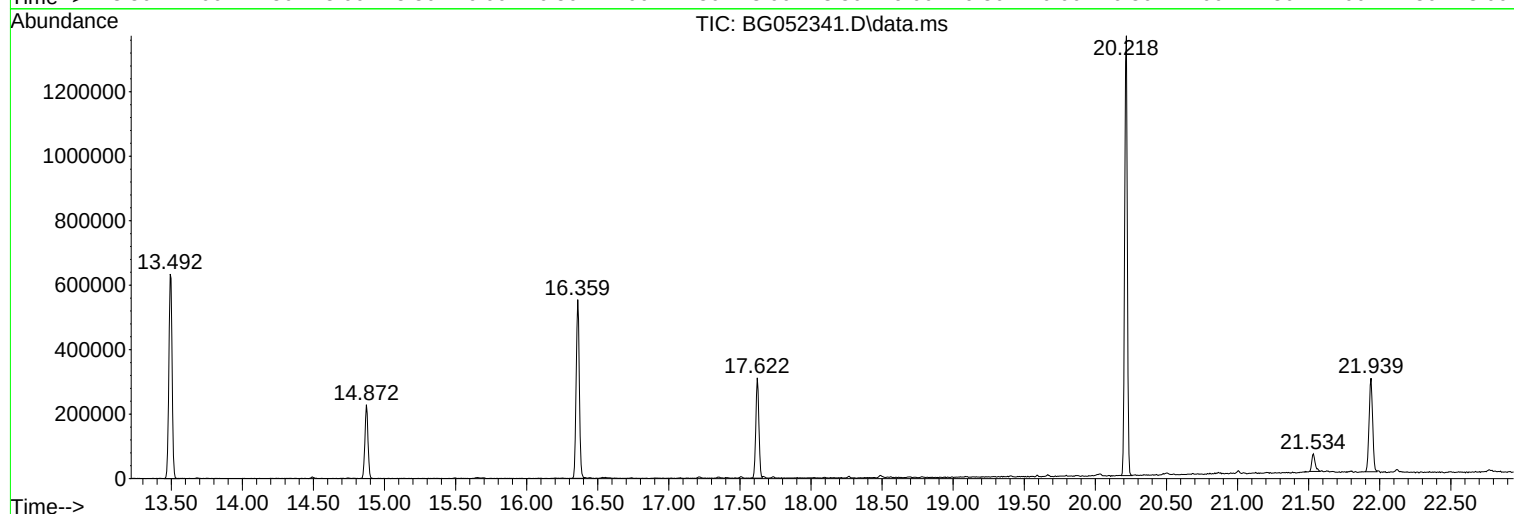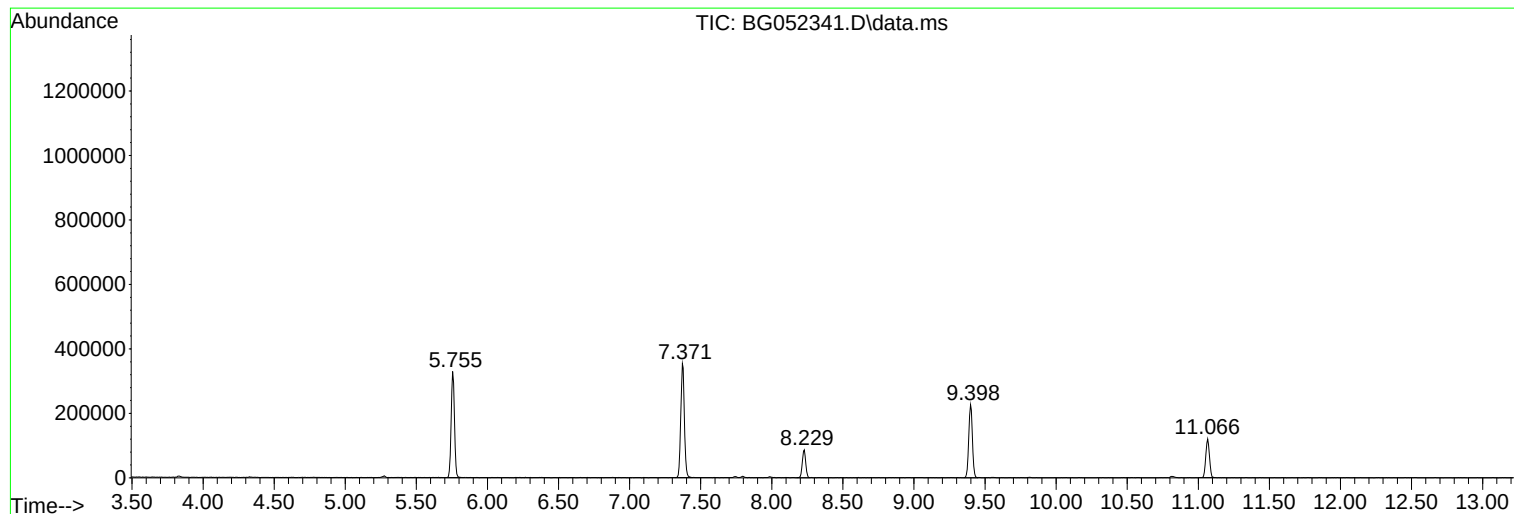

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020922\
Data File : BG052341.D
Acq On : 9 Feb 2022 19:00
Operator : CG/JU
Sample : N1432-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SP-3










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Trichloroacetic acid, hexad... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.534	3.70 ng	92186	Chrysene-d12	21.939

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	94
2			Pentadecafluorooctanoic acid, oc...	666	C26H37F15O2	1000406-04-8	91
3			2- Chloropropionic acid, octadec...	360	C21H41ClO2	088104-31-8	91
4			Trichloroacetic acid, pentadecyl...	372	C17H31Cl3O2	074339-53-0	91
5			1-Tetracosene	336	C24H48	010192-32-2	91

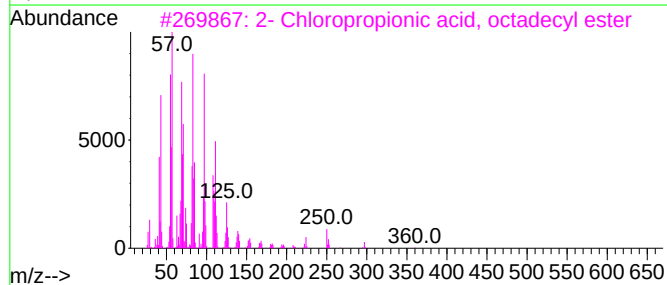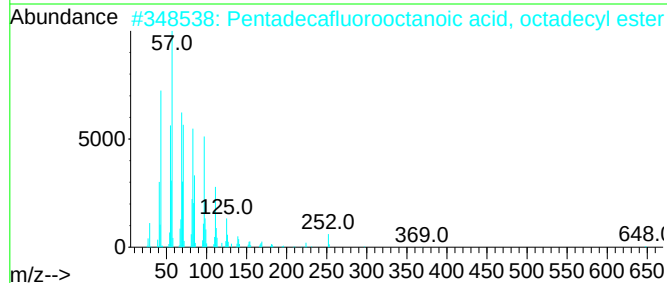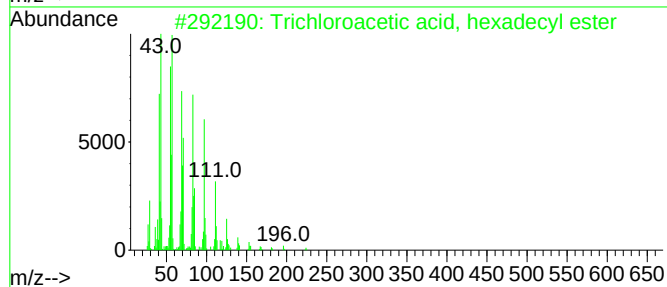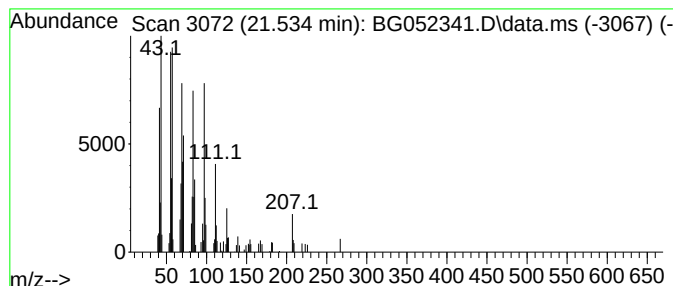

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020922\
Data File : BG052341.D
Acq On : 9 Feb 2022 19:00
Operator : CG/JU
Sample : N1432-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SP-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Trichloroacetic...	21.534	3.7	ng	92186	5	21.939	498326	20.0