

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020922\
 Data File : BG052346.D
 Acq On : 9 Feb 2022 22:11
 Operator : CG/JU
 Sample : N1424-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BLIND-DUPLICATE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG052346.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.755	379	386	396	rBV	394824	608587	29.05%	7.546%
2	7.371	654	661	673	rBV	407735	693977	33.13%	8.604%
3	8.223	800	806	813	rBV	76356	129324	6.17%	1.603%
4	9.397	998	1006	1014	rBV	244920	445681	21.28%	5.526%
5	11.066	1283	1290	1299	rBV	108578	193329	9.23%	2.397%
6	13.498	1696	1704	1712	rBV	713961	1077478	51.44%	13.359%
7	14.872	1931	1938	1947	rVB	204472	319525	15.25%	3.962%
8	16.359	2185	2191	2201	rBV	673243	1008278	48.14%	12.501%
9	17.622	2399	2406	2414	rBV	304297	462999	22.10%	5.740%
10	20.218	2842	2848	2853	rBV	1648821	2094608	100.00%	25.970%
11	21.534	3068	3072	3079	rVB8	13983	22322	1.07%	0.277%
12	21.939	3134	3141	3150	rVB2	296129	506846	24.20%	6.284%
13	25.417	3721	3733	3745	rVB2	161106	502587	23.99%	6.231%




Sum of corrected areas: 8065541

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020922\
Data File : BG052346.D
Acq On : 9 Feb 2022 22:11
Operator : CG/JU
Sample : N1424-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BLIND-DUPLICATE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

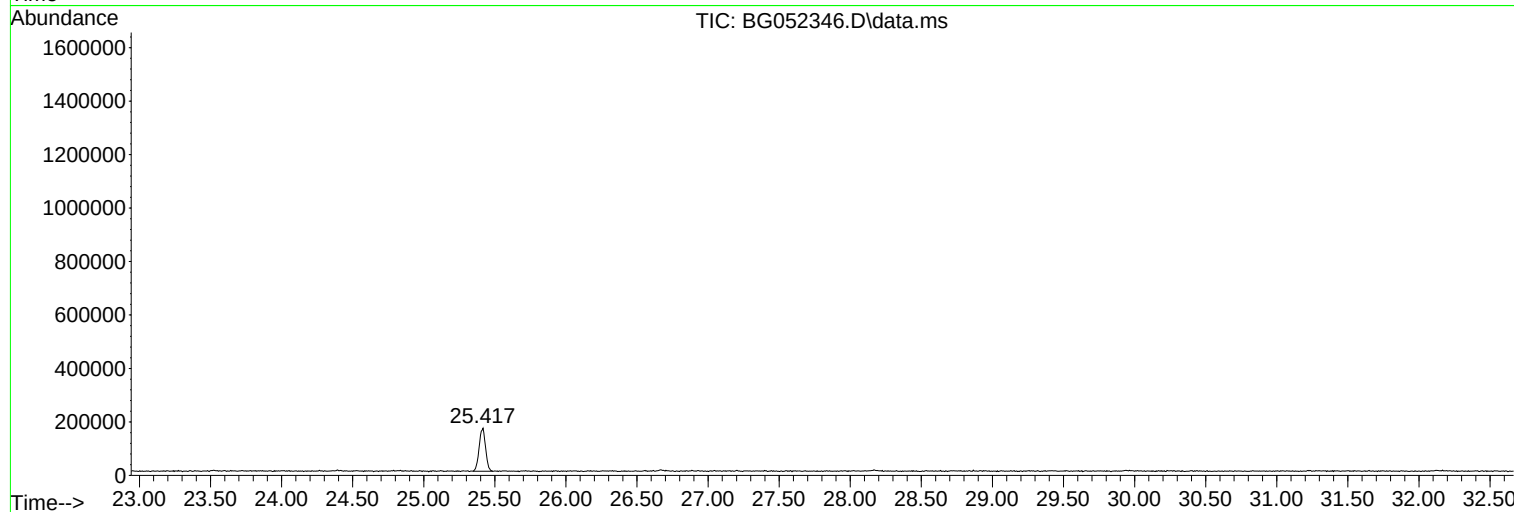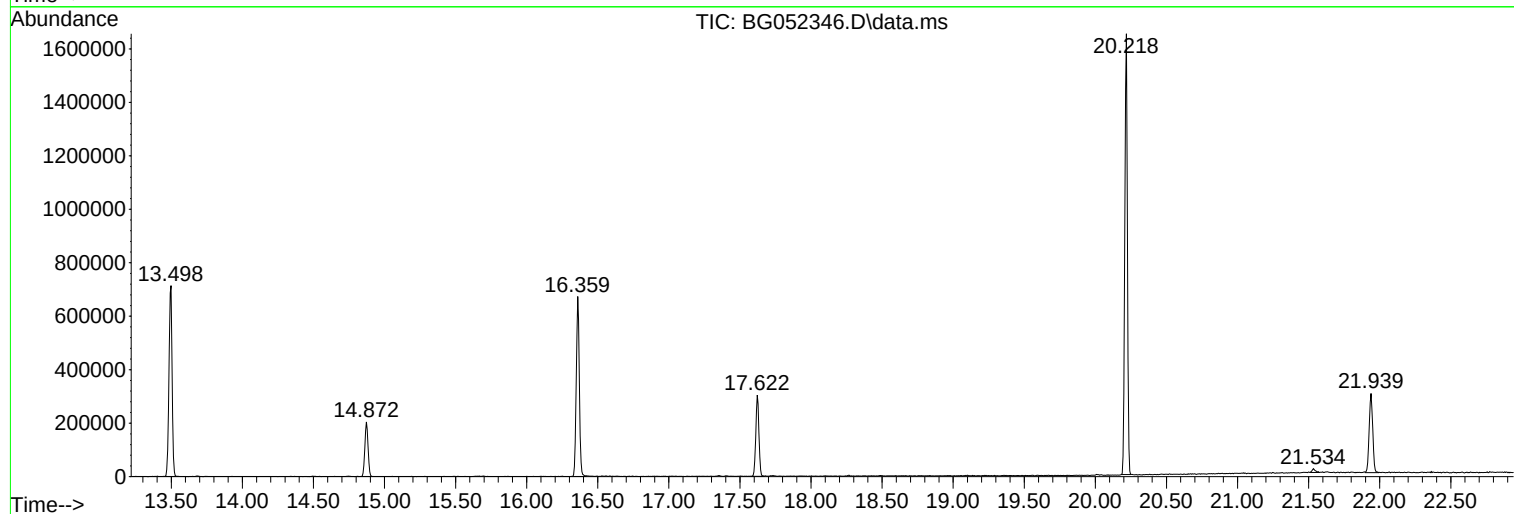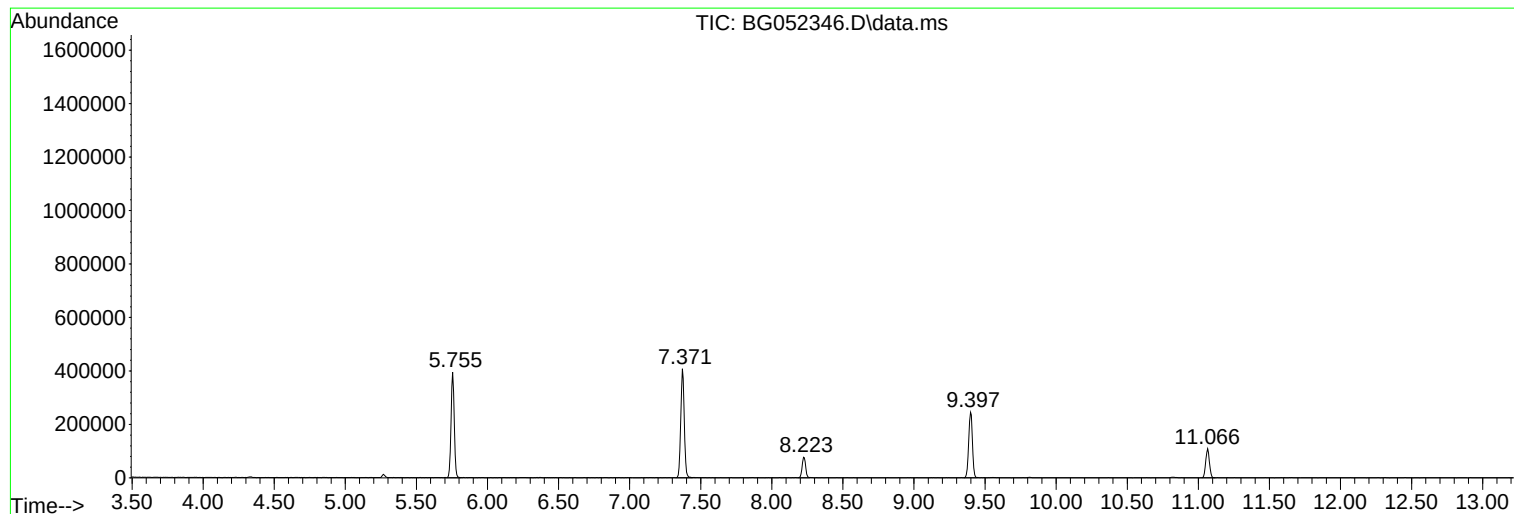

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020922\
Data File : BG052346.D
Acq On : 9 Feb 2022 22:11
Operator : CG/JU
Sample : N1424-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BLIND-DUPLICATE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020922\
Data File : BG052346.D
Acq On : 9 Feb 2022 22:11
Operator : CG/JU
Sample : N1424-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BLIND-DUPLICATE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------