
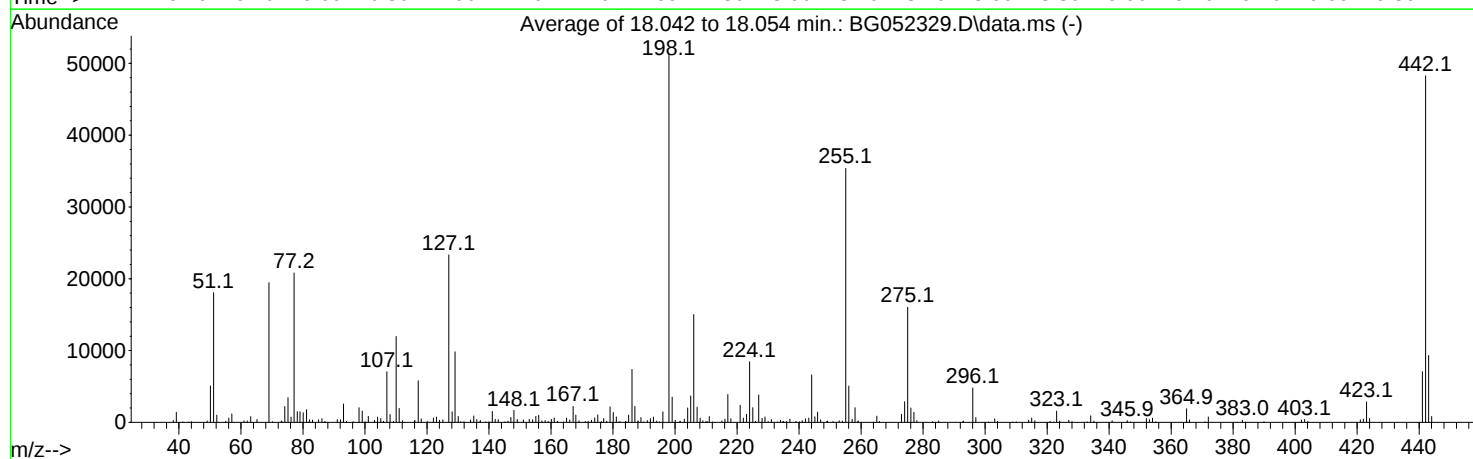


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020922\
 Data File : BG052329.D
 Acq On : 9 Feb 2022 10:37
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 08 01:21:20 2022

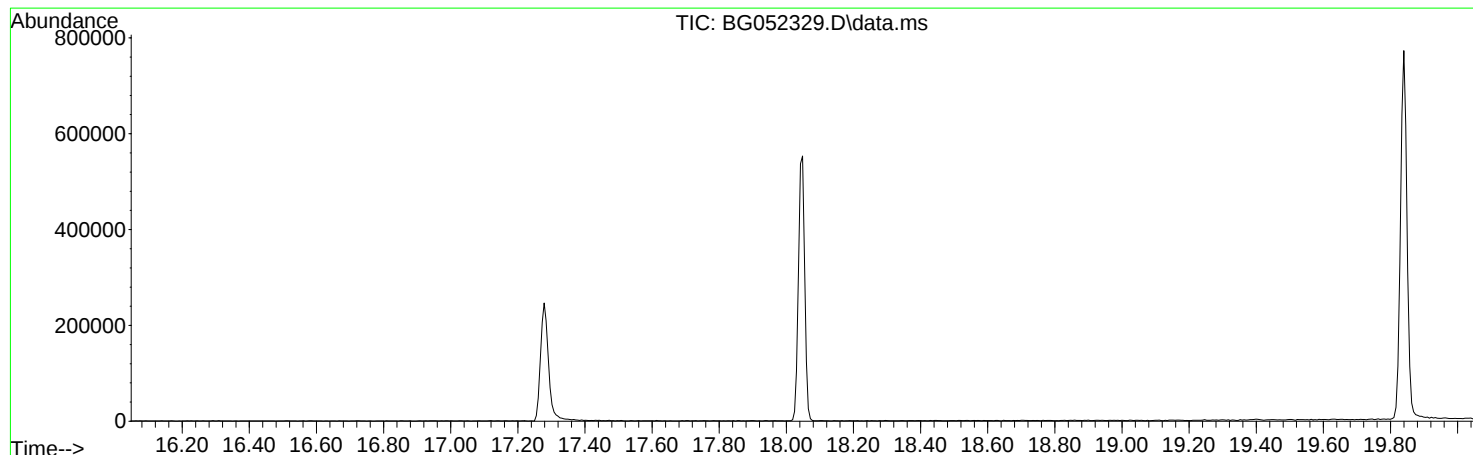

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	18075	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.0	19451	PASS
70	69	0.00	2	0.5	94	PASS
127	198	10	80	45.5	23332	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51237	PASS
199	198	5	9	6.9	3516	PASS
275	198	10	60	31.3	16030	PASS
365	198	1	100	3.7	1902	PASS
441	198	0.01	100	13.8	7072	PASS
442	442	50	100	100.0	48277	PASS
443	442	15	24	19.3	9314	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/9/2022	BNA_G	<u>BG052329.D</u>
Compound Name	Response	Retention Time
DDT	210470	21
DDD	2244	20.63
DDE	109	20.12
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2353	212823	1.11

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020922\
Data File : BG052329.D
Acq On : 9 Feb 2022 10:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 09 11:42:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 08 01:21:20 2022
Response via : Initial Calibration

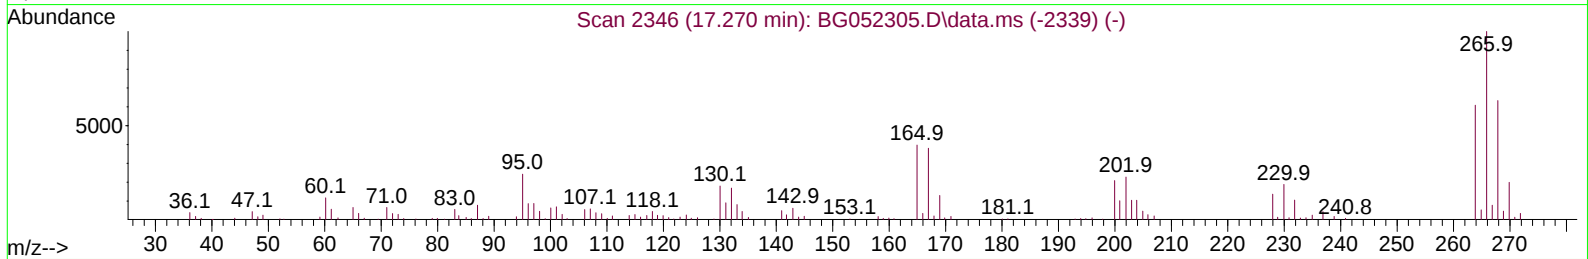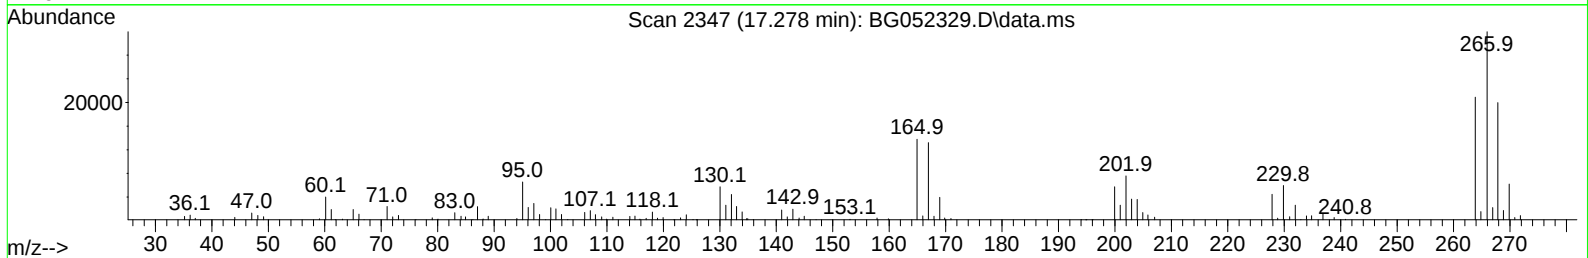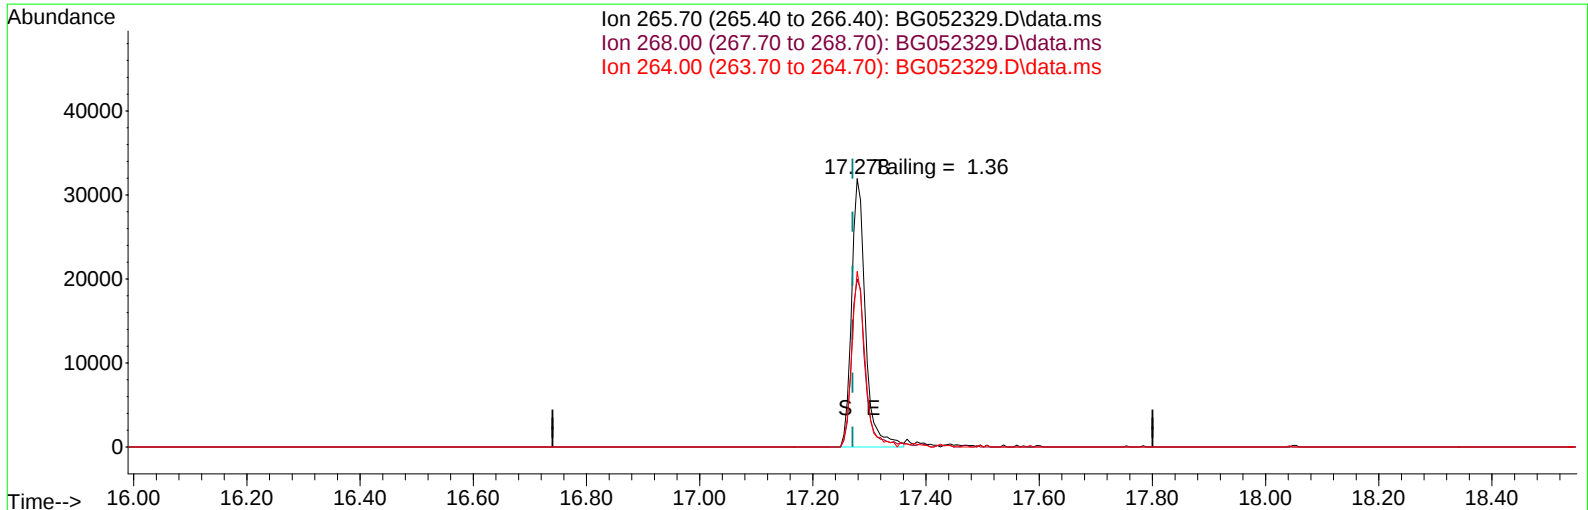

TIC: BG052329.D\data.ms

(70) Pentachlorophenol (C)

17.278min (+ 0.008) 22962.35 ng




response 54231

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	62.46
264.00	65.20	65.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG020922\
Data File : BG052329.D
Acq On : 9 Feb 2022 10:37
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 09 11:42:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 08 01:21:20 2022
Response via : Initial Calibration

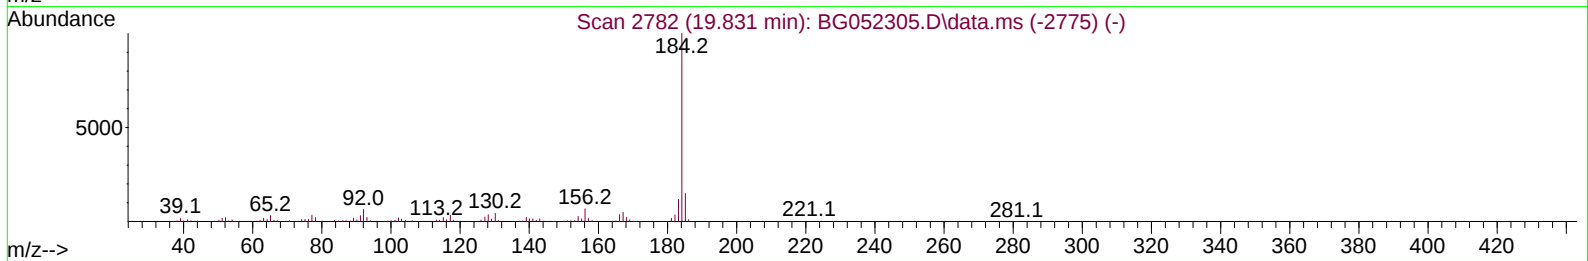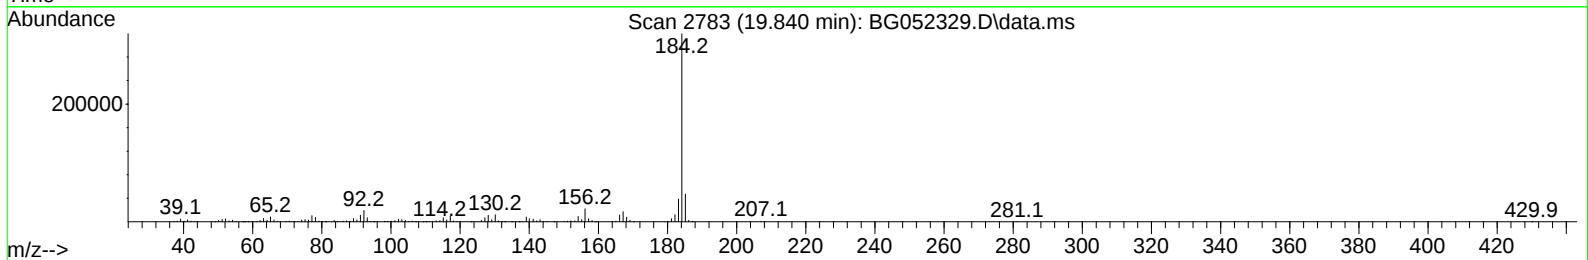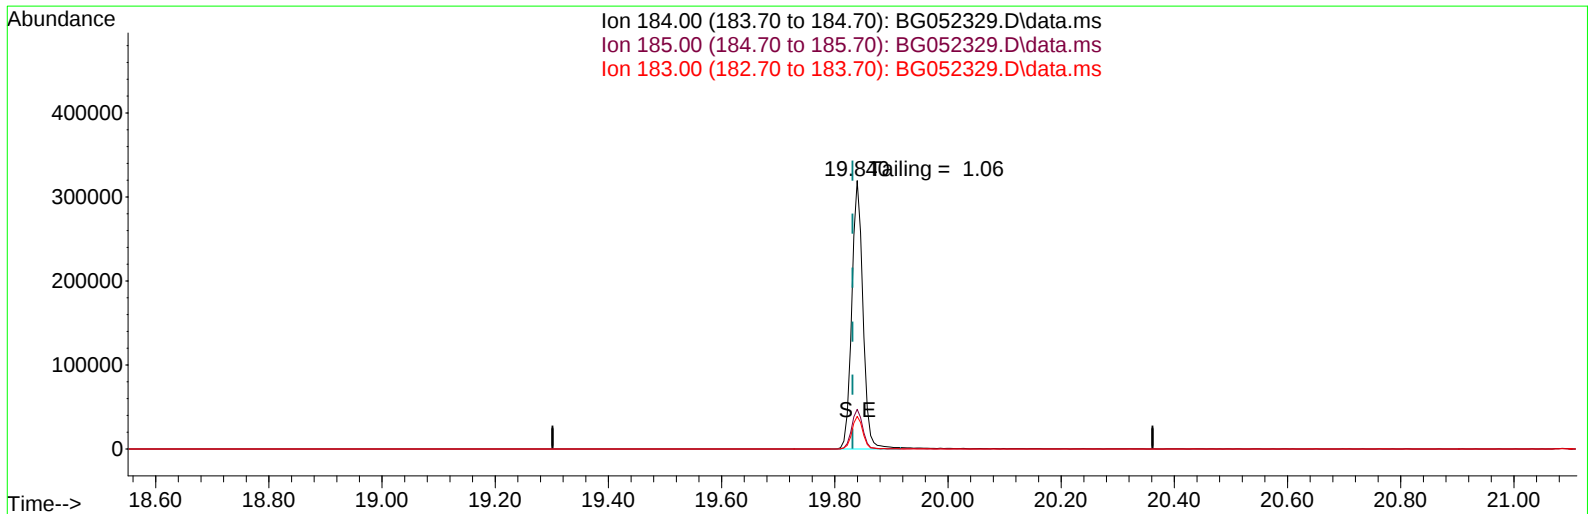

TIC: BG052329.D\data.ms

(77) Benzidine

19.840min (+ 0.009) 349965.80 ng m

response 433723

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.79
183.00	12.20	12.17
0.00	0.00	0.00